

AD-A027 099

USADAC TECHNICAL LIBRARY



5 0712 01015296 4

AD

Report 2165

OXYGEN FLASK METHOD FOR DETERMINING
ELEMENTS IN OILS - AN EVALUATION

TECHNICAL
LIBRARY

February 1976

Approved for public release; distribution unlimited.

U.S. ARMY MOBILITY EQUIPMENT
RESEARCH AND DEVELOPMENT COMMAND
FORT BELVOIR, VIRGINIA



Destroy this report when no longer needed.
Do not return it to the originator.

The citation in this report of trade names of commercially available products does not constitute official endorsement or approval of the use of such products.


UNCLASSIFIED

SECURITY CLASSIFICATION OF THIS PAGE (When Date Entered)

REPORT DOCUMENTATION PAGE		READ INSTRUCTIONS BEFORE COMPLETING FORM
1. REPORT NUMBER 2165	2. GOVT ACCESSION NO.	3. RECIPIENT'S CATALOG NUMBER
4. TITLE (and Subtitle) OXYGEN FLASK METHOD FOR DETERMINING ELEMENTS IN OILS - AN EVALUATION		5. TYPE OF REPORT & PERIOD COVERED Final
		6. PERFORMING ORG. REPORT NUMBER
7. AUTHOR(s) Marjan Kolobielski		8. CONTRACT OR GRANT NUMBER(s)
9. PERFORMING ORGANIZATION NAME AND ADDRESS Fuels and Lubricants Division, Lab 2000 U.S. Army Mobility Equipment Research and Development Command, Fort Belvoir, Virginia 22060		10. PROGRAM ELEMENT, PROJECT, TASK AREA & WORK UNIT NUMBERS 1F662611AH69
11. CONTROLLING OFFICE NAME AND ADDRESS		12. REPORT DATE February 1976
		13. NUMBER OF PAGES 22
14. MONITORING AGENCY NAME & ADDRESS (if different from Controlling Office)		15. SECURITY CLASS. (of this report) Unclassified
		15e. DECLASSIFICATION/DOWNGRADING SCHEDULE
16. DISTRIBUTION STATEMENT (of this Report) Approved for public release; distribution unlimited.		
17. DISTRIBUTION STATEMENT (of the abstract entered in Block 20, if different from Report)		
18. SUPPLEMENTARY NOTES		
19. KEY WORDS (Continue on reverse side if necessary and identify by block number)		
Phosphorus	Combustion	
Sulfur	Engine Oil	
Chlorine	Gear Oil	
Oxygen Flask	Spectroscopy	
20. ABSTRACT (Continue on reverse side if necessary and identify by block number)		
<p>The oxygen flask, combustion technique for determining phosphorus, sulfur, and chlorine in oils was evaluated using military lubrication oils as representative material. The concentration of those elements, after combustion of the samples, was determined spectrophotometrically. This technique is a rapid, simple, and inexpensive method for performing nonroutine analyses.</p>		

UNCLASSIFIED

SECURITY CLASSIFICATION OF THIS PAGE(When Data Entered)



UNCLASSIFIED

CONTENTS

Section	Title	Page
I	INTRODUCTION	
	1. Background	1
II	RESULTS AND DISCUSSION	
	2. Determination of Phosphorus	2
	3. Determination of Sulfur	3
	4. Determination of Chlorine	5
III	EXPERIMENTS	
	5. Apparatus	7
	6. General Combustion Procedure	7
	7. Safety Precautions	7
	8. Determination of Phosphorus	7
	9. Determination of Sulfur	9
	10. Determination of Chlorine	11
IV	CONCLUSIONS	
	11. Conclusions	12

OXYGEN FLASK METHOD FOR DETERMINING ELEMENTS IN OIL — AN EVALUATION

I. INTRODUCTION

I. **Background.** Military Laboratories are only equipped with apparatus suitable for performing quality surveillance tests of the supplied lubrication products according to military specifications.¹ These surveillance tests include the determinations of concentration of phosphorus, sulfur, and chlorine in individual lots. The military lubrication oils were selected for this study as representative products containing these elements. In addition, MERADCOM is engaged in research on these oils because it has the custodial responsibility for military automotive engine and gear-lubricating oils.²

The conformance tests for determination of these elements specify ASTM methods.³ These methods are reliable for routine analyses; however, they are often tedious and time-consuming and require special complex equipment which may be bulky and expensive. Military Laboratories need a rapid, simple, and inexpensive method for nonroutine determination of phosphorus, sulfur, and chlorine. Such a method could be incorporated into military specifications for lubricating oils.⁴ Ideally, this method should utilize readily available, portable, and unencumbering equipment.

The oxygen flask, combustion technique, originally developed by Schöniger,⁵ appeared promising for such applications.⁶ The combustion technique

- ¹ Military Specifications:
MIL-HDBK-200D, *Military Standardization Handbook*, "Quality Surveillance Handbook for Fuels, Lubricants, and Related Products," 1 March 1971.
MIL-L-50096A, *Laboratory, Petroleum, Base*, 30 Dec 1963.
MIL-L-51050A(G1), *Laboratory, Petroleum, Semitrailer Mounted*, 13 Dec 1965.
- ² Military Specifications:
MIL-L-2104C, *Lubricating Oil, Internal Combustion Engine, Tactical Service*, 20 Nov 1970.
MIL-L-46152, *Lubricating Oil, Internal Combustion Engine, Administrative Service*, 20 Nov 1970.
MIL-L-2105B, *Lubricating Oil, Gear, Multipurpose*, 19 Feb 1962.
- ³ *Annual Book of ASTM Standards*, American Society for Testing and Materials, Part 23, Philadelphia, PA (1975):
D1091-64, "Phosphorus in Lubricating Oils and Additives."
D129-64, "Sulfur in Petroleum Products (General Bomb Method)."
D1552-64, "Sulfur in Petroleum Products (High Temperature Method)."
D808-63, "Chlorine in New and Used Petroleum Products (Bomb Method)."
D1317-64, "Chlorine in New and Used Petroleum Products (Sodium Alcoholate Method)."
- ⁴ Military Specifications:
MIL-L-2104C, *Lubricating Oil, Internal Combustion Engine, Tactical Service*, 20 Nov 1970.
MIL-L-46152, *Lubricating Oil, Internal Combustion Engine, Administrative Service*, 20 Nov 1970.
MIL-L-2105B, *Lubricating Oil, Gear, Multipurpose*, 19 Feb 1962.
- ⁵ W. Schöniger, *Mikrochim Acta*, 1955, 123; 1956, 867.
- ⁶ C. Liddell, *J. Inst. Petrol.*, 48, 221 (1962).

consists of burning the sample, absorbed on a filter paper placed in a platinum gauze basket, in a glass flask filled with oxygen at atmospheric pressure and containing a suitable liquid absorbent. Combustion takes about 30 seconds. The elements present are then determined by suitable procedures. This technique was evaluated for determining phosphorus, sulfur, and chlorine content in oils using engine and gear-lubricating oils as representative materials. This report describes the results of the development and evaluation effort. The atomic absorption measurements were performed at MERADCOM by Mr. George Oswald.

II. RESULTS AND DISCUSSION

2. **Determination of Phosphorus.** Engine and gear-lubricating oils commonly contain organophosphorus-sulfur compounds and their derivatives as antioxidants, corrosion inhibitors, antiwear agents, and dispersant-detergents.⁷ In this study, the oxygen-combustion analysis for phosphorus was developed by modifying the Schöniger method^{8 9 10 11} and combining it with an ASTM spectroscopic procedure.¹² In this analysis, the sample is burned in the presence of sodium carbonate, and the combustion products containing sodium phosphate are absorbed in sulfuric acid. The phosphoric acid formed is then treated with an ammonium molybdate-hydrazine mixture to give the molybdenum blue complex. The absorbance of this colored compound, measured at 820 nm, is proportional to the concentration of phosphorus. The results of determination of phosphorus in oils are presented in Table I (tests 105, 106, 108, 109, and 110). The repeatability lies within the values recommended by the standard phosphorus oxidation method, ASTM D1091.¹³ Also, the deviation of the mean from the value obtained by the ASTM method is small. Other elements, usually present in most lubricating oils, did not interfere in this procedure. The capsule, employed in other methods as a sample carrier,^{14 15} was not used here. It was found that the capsule material, gelatine and cellulose acetate, contained phosphorus and, therefore, would distort the results (Table I, test 115).

⁷ M. Kolobielski, *Determination of Zinc Dialkyl (Diaryl) Dithiophosphate in Lubricating Oil*, AD757605, Feb 1973.

⁸ K. D. Fleischer, *et al.*, *Anal. Chem.*, 30, 152 (1958).

⁹ J. E. Barney II, *et al.*, *Anal. Chem.*, 31, 1394 (1959).

¹⁰ S. J. Gedansky, *et al.*, *Anal. Chem.*, 32, 1447 (1960).

¹¹ "Proposed Methods for Petroleum and Petroleum Products," Appendix IV, American Society for Testing and Materials, Philadelphia, PA, 1965.

¹² "Annual Book of ASTM Standards," American Society for Testing and Materials, Part 25, Philadelphia, PA, Test D3231, 1975.

¹³ "Annual Book of ASTM Standards," American Society for Testing and Materials, Part 23, Philadelphia, PA, Test D1091-64, 1975.

¹⁴ S. J. Gedansky, *et al.*, *Anal. Chem.*, 32, 1447 (1960).

¹⁵ "Proposed Methods for Petroleum and Petroleum Products," Appendix IV, American Society for Testing and Materials, Philadelphia, PA, 1965.

Table I. Determination of Phosphorus

Test No.	Material	Elements Present	% Phosphorus		Mean
			By ASTM D1091	By Proposed Method	
105	Engine Oil: MIL-L-45199B	P,S,Ca,Ba,Zn, C,H,O,N	0.052	0.060	0.061
106	"	"	"	0.059	
108	"	"	"	0.064	
109	Gear Oil: MIL-L-2105B	P,S,Cl,C,H,O	0.060	0.058 0.062	0.060
110	"	"	0.110	0.112 0.110	0.111
115	Gelatine Capsule Cellulose Acetate	P,C,H,O "	—	0.013 0.071	

3. **Determination of Sulfur.** Several methods employing the oxygen-combustion technique have been reported. All these methods have a similar combustion procedure for sulfur, present in the organic compound, as the first stage. The first stage results in the formation of sulfuric acid. These methods differ only in the way of determining the sulfuric acid. The simplest method, employed by many authors, involves a variety of titrimetric procedures: with sodium hydroxide in the presence of methyl red,^{16 17 18 19} with standard barium chloride solution in the presence of Sulfonazo III indicator,²⁰ or with barium perchlorate in the presence of Thorin^{21 22} and Arsenazo III indicators.²³

¹⁶ I. Lysy and J. E. Zarembo, *Anal. Chem.*, **30**, 428 (1958).

¹⁷ C. Liddell, *J. Inst. Petrol.*, **48**, 221 (1962).

¹⁸ N. H. Furman, *Standard Methods of Chemical Analysis*, D. Van Nostrand, Co., Inc., New York, N.Y., p. 1014 (1966).

¹⁹ A. R. Crawford and G. V. Dyroff, "An Evaluation of Methods for Determining Sulfur in Fuel Oils," Air Pollution Control Association 63rd Annual Meeting, Paper 70-46 (June 1970).

²⁰ "Annual Book of ASTM Standards," American Society for Testing and Materials, Part **30**, Philadelphia, PA, Test E443-74 (1975).

²¹ D. B. Ratcliffe and A. T. S. Cunningham, *Fuel*, **47**, 89 (1968).

²² L. H. Scroggins, *J. Assoc. Official Anal. Chem.*, **56**, 892 (1973).

²³ S. M. Ahmed and B. J. P. Whalley, *Fuel*, **48**, 217 (1969); **51**, 190 (1972).

A spectroscopic method has also been suggested.^{24 25} It consists of reacting the sulfuric acid with barium chloranilate in a buffered solution of pH 4.3 and then determining the liberated chloranilic acid by measuring its absorbance at 330 nm. In another spectroscopic method, the sulfuric acid formed is reacted with a known amount of barium chloride solution, and the excess of barium is determined by atomic absorption spectroscopy.²⁶ Still another method suggests reacting the sulfuric acid with a known and excessive amount of barium bromate to produce a precipitate of barium sulfate. The excess of barium bromate is determined iodometrically.²⁷

The first three methods were investigated in this study. The results are presented in Table 2. The titrimetric method was tested on a sulfur standard containing an organosulfur compound in a hydrocarbon oil (tests 176, 176a, and 177) and on a formulated lubricating oil containing phosphorus, calcium, barium, and zinc in addition to carbon, hydrogen, oxygen, sulfur, and nitrogen. The titration of the product, obtained upon combustion of the sulfur standard, gave values close to those expected. However, the results from the lubricating oil were too high because of formation of phosphoric, in addition to sulfuric, acid during the combustion and oxidation reaction.

The spectroscopic method with barium chloranilate was applied to a sulfur standard solution (test 10), engine oils (test 11), and gear oils (test 12). The duplicate values in each test were close, and the deviation of the mean from the expected value was also small in tests 10 and 11. In the case of gear oil (test 12), the deviation was too high. It was not established if the error lay in this method or was due to a mistaken value reported by the laboratory which performed the standard determination of sulfur by the bomb method (ASTM D129).²⁸

In the method where barium excess was determined by atomic absorption spectroscopy, the measurements were done at 455 and 554 nm. In the case with the higher wavelength, potassium acetate was added to the solution to suppress the ionization of barium. The duplicate results and the means are close to the values given for the standard solutions (tests 26, 22, and 21) or determined by other methods (tests 17, 27, 28, and 17a). In both spectroscopic methods (with barium chloranilate and atomic absorption spectroscopy, no interference by metals or phosphorus was observed.

²⁴ R. J. Bertolacini and J. E. Barney II, *Anal. Chem.*, 29, 281 (1957).

²⁵ R. W. Klipp and J. E. Barney II, *Anal. Chem.*, 31, 596 (1959).

²⁶ H. W. Lautenbacher and H. W. Baker, *Amer. Laboratory*, 4, No. 8, 45 (1972).

²⁷ Y. A. Gawargious and A. B. Farag, *Talanta*, 19, 641 (1972).

²⁸ "Annual Book of ASTM Standards," American Society for Testing and Materials, Part 23, Philadelphia, PA, Test D129-64, 1975.

Table 2. Determination of Sulfur

Test No.	Material	Elements Present	% S By Other Method	Procedure of Proposed Method	% S	
					By Proposed	Method Mean
176	Standard	S,C,H	1.0305	Titrimetric	0.9984	
177	"	"	"	"	0.8030	0.9013
					0.9024	
176a	"	"	0.9893	"	0.786	0.849
					0.887	
					0.873	
175	Engine Oil: MIL-L-45199B	S,P,Ca, Ba,Zn,C,H,O,N	0.390 (ASTM D129)	"	0.510	
10	Standard	S,C,H,	0.1989	Barium Chlor- anilate	0.1575	0.1720
					0.1864	
11	Engine Oil	as in 175	0.390 (ASTM D129)	"	0.4137	0.3960
					0.3783	
12	Gear Oil: MIL-L-2105B	S,P,Cl, C,H,O	0.370 (ASTM D129)	"	0.2295	0.2518
					0.2741	
26	Standard	S,C,H	0.1989	AAS,* at 554 nm	0.165	0.1910
					0.217	
22	"	"	0.9893	"	0.973	1.0100
					1.047	
17	Engine Oil	as in 175	0.39	"	0.29	0.32
					0.35	
27	"	S,P,Ca,Ba,Zn,C, H,O,N	0.46 (ASTM D129)	"	0.442	0.432
					0.421	
28	"	"	0.27 (ASTM D129)	"	0.197	0.215
					0.232	
21	Standard	S,C,H,O	0.9893	AAS, at 455 nm	0.951	0.928
					0.904	
17a	Engine Oil	as in 175	0.39	"	0.38	0.395
					0.41	

* Atomic Absorption Spectroscopy.

4. **Determination of Chlorine.** Several methods were reported for the determination of chlorine by the oxygen flask technique. One simple method involves reaction of the chloride, formed upon combustion, with mercuric chloranilate in 0.05 N nitric acid and determination of the absorbance of the liberated chloranilic acid at 306 nm.²⁹ The chloride can also be determined by amperometric,³⁰ or potentiometric titration with silver nitrate solution,^{31 32 33} atomic absorption,³⁴ compleximetric

²⁹ J. E. Barney II and R. J. Bertolacini, *Anal. Chem.*, 29, 1187 (1957); 30, 202 (1958).

³⁰ D. B. Ratcliffe and T. L. Young, *Fuel*, 47, 185 (1968).

³¹ "Annual Book of ASTM Standards," American Society for Testing and Materials, Part 30, Philadelphia, PA, Test E-442 (1975).

³² M. Corner, *Analyst*, 84, 41 (1959).

³³ J. Haslam, *et al.*, *Analyst*, 85, 556 (1960).

³⁴ E. D. Truscott, *Anal. Chem.*, 42, 1657 (1970).

titration,³⁵ or titration with mercuric nitrate.³⁶

The spectroscopic method, with mercuric chloranilate, was employed here for chlorine determination of a chlorine standard, a gear oil, and an oil additive (Table 3). The standard chlorine solution was analyzed in duplicate, and the analyses were replicated on different days (tests 187, 188, and 189). Samples of a gear oil (tests 185 and 191) and an oil additive (test 3) were also analyzed under the same conditions. All these results indicate that the repeatability of this method is good and its value lies within the repeatability value (0.07% for materials with 0.1 to 2% chlorine content) recommended by another method involving a bomb oxidation technique.³⁷ In these tests, the deviation of the mean values from the corresponding values determined by other methods and other laboratories was relatively small. Since it was reported that metals interfere in this spectroscopic method,³⁸ a test was performed in which the cations were removed from the combustion product by treatment with an ion exchange resin (test 2). The mean chlorine content was much closer to the expected value than the chlorine content obtained in tests without the treatment (tests 185 and 191).

Table 3. Determination of Chlorine

Test No.	Material	Elements Present	% CL By Other Method	Procedure of Proposed Method	% CL	
					By Proposed Method	Mean
187	Standard	Cl,C,H	0.899	Regular	0.847 0.771	0.809
188	"	"	"	"	0.698 0.781	0.740
189	"	"	"	"	0.890 0.851	0.870
185	Gear Oil: MIL-L-2105B	Cl,S,C,H,O	1.49 (ASTM D808)	"	1.09 1.07	1.08
191	"	"	"	"	1.12 1.18	1.15
3	Standard prepared from extreme pressure gear oil additive	Cl,S,C,H,O	0.6037 (ASTM D808)	"	0.692 0.623	0.657
2	Gear Oil	as in 185	1.49	with ion ex- change resin	1.23 1.25	1.24

³⁵ J. Z. Falcon, *et al.*, *Anal. Chem.*, 47, 171 (1975).

³⁶ N. P. Sosnina and T. N. Krasnova, *Khimiia i Tekhnologiia Topliv i Masel*, 17, 49 (1972).

³⁷ "Annual Book of ASTM Standards," American Society for Testing and Materials, Part 23, Philadelphia, PA, Test D808-63 (1975).

³⁸ J. E. Barney II and R. J. Bertolacini, *Anal. Chem.*, 29, 1187 (1957); 30, 202 (1958).

III. EXPERIMENTS


5. **Apparatus.** The apparatus is shown in the figure (page 8). The main parts are: 500- to 1000-ml conical flask of borosilicate glass with a spherical joint and a flaring lip; glass stopper with a hook and a spherical ground joint; platinum gauze basket as a sample carrier; pinch clamp; safety metal cabinet with transparent plastic door and inclined platform for the flask; and infrared light igniter with a cord and a line switch for remote firing.

6. **General Combustion Procedure.** The black paper sample wrapper (sample area 32 by 30 mm, with "fuse" 8 by 38 mm) is folded to form a cup and then placed in the platinum carrier with the "fuse" projecting. The sample carrier with the paper is tared, and the sample (10 to 50 mgs) is introduced into the paper cup. The platinum carrier is suspended on the hook of the stopper, and the latter is set aside. The combustion flask is first charged with a suitable absorbent and then filled, for about 3 to 4 minutes, with oxygen which is passed in through a delivery tube reaching nearly to the bottom of the flask. The stopper with the sample in the platinum carrier is inserted into the flask and secured with the pinch clamp. The flask is placed on the inclined platform inside the metal cabinet. The flask is positioned within the chamber by adjusting the crank handle and the platform so that the focal point of the lamp beam (1.5 inches in front of the red filter) is on the black paper "fuse." The remote firing is performed by means of the line switch which is located 4 feet from the cabinet. After the combustion is complete, the flask is allowed to cool for about 1 minute, then the platinum basket is dropped into the absorbent, and the flask is well shaken in order to absorb the combustion products. Further procedures vary with particular element determination. A procedure blank is run simultaneously with each sample. The blank consists of reagents to which no unknown sample is added.

7. **Safety Precautions.** Many combustions have been carried out without mishap. However, the following precautions should be exercised. The combustion flask must not contain any residue or vapors of organic solvents which may produce a violent explosion upon ignition. The combustion must be carried out in a hood in the safety cabinet. The operator should wear goggles, face shield, and gloves for protection during the combustion operation.

8. **Determination of Phosphorus.**

a. **Procedure.** The unknown oil sample is weighed on to 0.03 g of sodium carbonate in the black paper wrapper cup prior to combustion and then covered with an additional 0.02 g of Na_2CO_3 . The absorbent used, 10 percent sulfuric acid, is

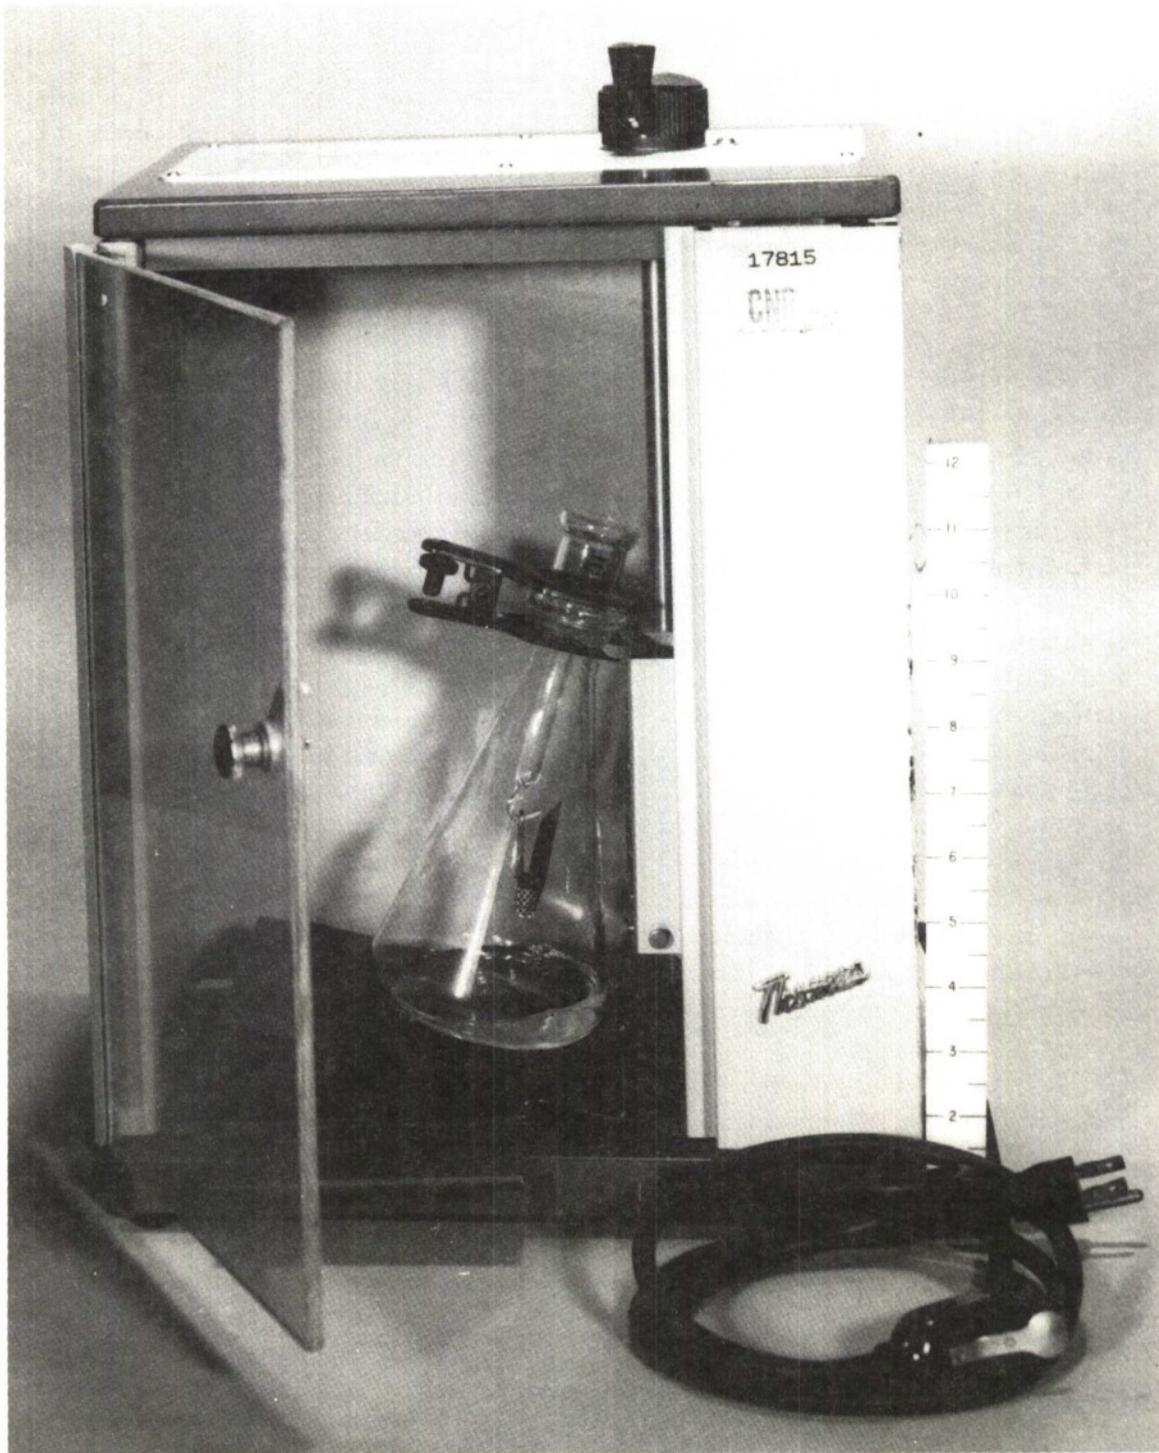

Combustion Assembly

placed in the combustion flask. After the combustion is completed, the flask is intermittently shaken, and then the stopper is washed down with distilled water. A freshly prepared 50 ml of molybdate-hydrazine reagent is added, and the mixture is transferred to a 100-ml volumetric flask. The combustion flask is rinsed with water, the washings are added to the volumetric flask, and the solution is diluted to 100 ml with water and mixed well. After the solution is mixed, the stopper is removed, and the flask is placed in a water bath (71 to 99° C) for 25 minutes. The flask is then cooled to room temperature, and the absorbance of the blue-colored complex is measured at 820 nm in a 1-cm cell using distilled water in the reference cell. The absorbance of the unknown sample solution is corrected by subtracting the absorbance of the blank. The concentration of phosphorus is determined by comparing the corrected absorbance of the unknown sample with the calibration curve.

b. **Molybdate-Hydrazine Reagent.** A 20-g sample of ammonium molybdate tetrahydrate ($(\text{NH}_4)_6\text{MO}_7\text{O}_{24} \cdot 4\text{H}_2\text{O}$) is dissolved in a solution of concentrated sulfuric acid (225 ml) in water (500 ml). Next, the solution is transferred to a 1000-ml flask and diluted to the mark with water. In another 1000-ml flask, hydrazine sulfate ($\text{H}_2\text{NNH}_2 \cdot \text{H}_2\text{SO}_4$, 1.5g) is dissolved in 1ℓ of water. The reagent is prepared by mixing 25 ml of ammonium molybdate solution with 10 ml of hydrazine sulfate solution in a 100-ml volumetric flask and diluting to the mark with water. The reagent is unstable and should be used within 4 hours.

c. **Calibration Curve.** A 4.3930-g sample of dry potassium dihydrogen phosphate (KH_2PO_4) is dissolved in 150 ml of 10% sulfuric acid in a 1000-ml flask and diluted to the mark with water. A 10-ml sample of this solution is then diluted with water to 1000-ml volume to give a standard phosphorus solution of 10.0 μg phosphorus per ml. Exact amounts of the standard solution (0, 1.0, 2.0, 3.0, and 4.0 ml) are transferred into 100-ml volumetric flasks. This is followed by addition of 10 ml of 10% sulfuric acid, 50 ml of molybdate-hydrazine reagent, and then water to the 100-ml mark. These phosphorus solutions are submitted to the same sequence of operations as the unknown sample – heating, cooling, and measuring the absorbance. The calibration curve is obtained by subtracting from each absorbance the absorbance of the 0-ml phosphorus standard and plotting these corrected absorbances against the concentration of phosphorus in each standard solution (in μg per ml).

9. Determination of Sulfur.

a. **Titrimetric Procedure.** The oil sample (0.02 to 0.05 g) is weighed directly on to the black paper folded wrapper. The flask is charged with 10 ml of 3% hydrogen peroxide solution. After combustion, the solution is boiled gently to remove carbon dioxide and to destroy hydrogen peroxide. Then, it is cooled and titrated with 0.02 N sodium hydroxide solution in the presence of methyl red indicator. The

volume of the titrant used in the blank titration is subtracted from that of the unknown sample.

b. **Spectroscopic Procedure with Barium Chloranilate.** The weighing and combustion stages are similar to those described above. After combustion and heating, the flask content is transferred to a 100-ml volumetric flask. Ethanol (95%, 50 ml) is then added, followed by 10 ml of the buffer solution, water to the mark, and 0.3 g of solid barium chloranilate. The volumetric flask is shaken for 15 minutes, and then the content is filtered through Whatman No. 42 filter paper to remove the excess of barium reagent. The absorbance of the filtrate is measured at 330 nm in a 1-cm cell against the reagent blank (50% of 95% C_2H_5OH + 10% of buffer solution + 40% of water) in the reference cell. This absorbance is corrected by subtracting from the measured value the absorbance of the blank. The concentration of sulfur is determined by comparing the corrected absorbance of the unknown sample with the calibration curve.

The buffer (pH 4.3) required in the reaction is an aqueous solution of 0.02 M concentration of both acetic acid and sodium acetate. To obtain the calibration curve, a 2.06057-g sample of anhydrous ammonium sulfate is dissolved in 100 ml of water. A 10-ml sample of this solution is then diluted with water to 1000-ml volume to give a standard sulfur solution of $5 \mu\text{g}$ of sulfur per ml. Exact amounts of the standard solution (5, 10, 15, 20, 25, and 30 ml) are added separately to 100-ml volumetric flasks. This is followed by addition to each flask of the following materials: 10 ml of buffer solution, 50 ml of 95% ethanol, water up to the 100-ml mark, and 0.3 g of barium chloranilate. These sulfur solutions are submitted to the same sequence of operations as the unknown sample – shaking, filtering, and measuring the absorbance against the reagent blank in the reference cell. Finally, the absorbance is plotted against the sulfur concentration to give the calibration curve.

c. **Spectroscopic Procedure with Barium Chloride.** The oil sample (20 to 50 mg) is weighed on to the folded black wrapper which is then wetted with two drops of water to reduce the combustion rate and to minimize soot formation. The combustion flask contains 20 ml of barium chloride solution of known concentration (for example, 50 ppm Ba) and a few drops of 30% hydrogen peroxide. After combustion, the flask is shaken and then allowed to stand for 20 minutes. It is again shaken, and the solution is transferred to a 7-dram glass vial. The vial is cooled in an ice-bath and centrifuged at 1500 rpm for 30 minutes. The supernatant fluid is aspirated into the atomic absorption spectrophotometer without disturbing the centrifugate. The absorbance of the solution is measured at 455 nm or 554 nm. In the latter case, potassium acetate (0.25 g CH_3COOK per 100 ml) is added to the combustion flask. The sulfur content is calculated from the formula:

$$\% S = \frac{(\text{ppm Ba used} - \text{ppm Ba blank}) \times 20 \times 0.02335}{\text{weight of sample, in mg}}$$

(using 20-ml volume of a standard barium solution).

The standard barium solutions (10, 20, 40, 50, 75, 100, 250 ppm Ba) are prepared by dissolving an 0.8895-g sample of $\text{BaCl}_2 \cdot 2\text{H}_2\text{O}$ in 500 ml water and then taking measured volumes of this stock solution and diluting them with water to exact volumes in volumetric flasks. The "ppm Ba used" is the difference between the barium concentration of the standard barium chloride solution (in the 20-ml sample) and the concentration in the supernatant fluid, after the reaction, as determined by the atomic absorption spectrophotometry.

10. Determination of Chlorine. The oil sample (10 to 50 mg) is weighed on to the folded black paper. The combustion flask contains 5 ml of 0.1 N sodium hydroxide solution and 5 ml of 3% hydrogen peroxide. After the combustion is completed, the solution is boiled for a few minutes on a hot plate and then cooled. The content is transferred to a 100-ml volumetric flask and treated with 5 ml of 1 N nitric acid and 50 ml of Methyl Cellosolve and completed with water to the mark. Mercuric chloranilate (0.2 g) is then added, the flask is shaken for 15 minutes, and the excess of the mercuric reagent is removed by filtration through Whatman No. 42 filter paper. The absorbance of the filtrate is measured at 306 nm in a 1-cm cell against a reagent blank in the reference cell (filtrate from: 5 ml 1 N HNO_3 , 50 ml Methyl Cellosolve, 45 ml water, and 0.2 g mercuric chloranilate). The absorbance is corrected by subtracting from the measured value the absorbance of the blank. The chloride concentration is then obtained by comparing the corrected absorbance with the calibration curve prepared from standard ammonium chloride solution. In those cases when interfering cations (Ba, Ca, Pb, Zn) are present in the unknown sample, they are removed by using the ion exchange resin, Amberlite IR-120, hydrogen form. The regular procedure is modified by adding 0.5 g of this resin to the combustion flask after the combustion is completed. The mixture is filtered through S and S No. 589 filter paper, and the filtrate is transferred to a 100-ml flask. Further operation sequence follows the regular procedure.

The standard ammonium chloride solutions (0.04-, 0.10-, 0.20-, 0.40-, and 0.60-mg chloride per 100 ml) are made by diluting the standard stock solution (1.5105 g of ammonium chloride in 1000 ml water). A sample of each standard solution of known concentration is treated the same way as the known chlorine-containing material. The sample is admixed with 5 ml 1 N HNO_3 , 50 ml Methyl Cellosolve, completed with water to the 100-ml mark, and then treated with 0.2 g of mercuric chloranilate in a 100-ml flask. After filtration, the absorbance of each filtrate is measured at

306 nm, and the values are plotted against the chloride concentration to give the calibration curve.

IV. CONCLUSIONS

11. **Conclusions.** This study was concerned, mainly, with the evaluation of the oxygen-combustion method as a novel technique for potential use by the Military Laboratories. Specifically, this technique was considered for potential inclusion in military specifications for automotive lubricating oils. The short duration of this study did not generate sufficient data for performing a statistical analysis to determine the precision of these analytical methods. However, it is apparent that the oxygen flask, combustion method is a rapid, simple, and inexpensive laboratory technique for determining such elements as phosphorus, sulfur, and chlorine present in military oils and related products.

Among the different procedures tested on the samples containing sulfur and chlorine, the methods which involve barium chloranilate for sulfur and mercury chloranilate with ion exchange resin for chlorine appear to be the most reliable.

DISTRIBUTION FOR MERADCOM REPORT 2165

No. Copies	Addressee	No. Copies	Addressee
	Department of Defense		Department of the Army
1	Director, Technical Information Defense Advanced Research Projects Agency 1400 Wilson Blvd Arlington, VA 22209	9	Commander US Army Materiel Development and Readiness Command ATTN: DRCRD-WB DRCRD-F DRCRD-J DRCRD-ES DRCRD-GP DRCPA-E DRCRD-TC DRCSU-L DRCRD-O 5001 Eisenhower Ave Alexandria, VA 22333
1	Director Defense Nuclear Agency ATTN: APTL Washington, DC 20305		
12	Defense Documentation Center Cameron Station Alexandria, VA 22314	1	Commander, HQ TRADOC ATTN: ATEN-ME Fort Monroe, VA 23651
1	Commander DCASR St. Louis ATTN: DCRS-QT 1136 Washington Ave St Louis, MO 63136	1	HQDA (DAEN-RDO) Washington, DC 20314
		2	HQDA ATTN: DAMA-ARZ-B DALO-SMZ-L Washington, DC 20310
1	Office, Chief of Res & Dev Room 3D424 ATTN: DARD-DDC Washington, DC 20310	1	HQDA (DAEN-MER-M) Washington, DC 20314
1	OACSFOR DAFD-SDS The Pentagon Washington, DC 20310	1	HQDA (DAEN-MCE-D) Washington, DC 20314
		2	Commander US Army Missile Research and Development Command ATTN: DRSMI-RSM DRSMI-RRS Redstone Arsenal, AL 35809
3	Defense Fuel Supply Center Office of Technical Services ATTN: DFSC-T Cameron Station Alexandria, VA 22314	1	Chief, Engineer Division DCSLOG ATTN: AFKC-LG-E HQ Sixth US Army Presidio of San Francisco, CA 94129
1	Director of Defense Research and Engineering (OSD) ATTN: Dep Dir/Research and Technology Washington, DC 20301	1	Asst Chief of Staff for Communications-Electronics ATTN: DACE-EDC-E Washington, DC 20314

No. Copies	Addressee	No. Copies	Addressee
2	Director Army Materials and Mechanics Research Center ATTN: DRXMR-STL DRXMR-MS Technical Library Watertown, MA 02172	5	Commander US Army Troop Support and Aviation Materiel Readiness Command ATTN: DRSTS-KTE DRSTS-O DRSTS-RE DRSTS-RT DRSTS-DRL 4300 Goodfellow Blvd St Louis, MO 63120
1	US Army Ballistic Research Laboratories Technical Library DRXBR-LB (Bldg 305) Aberdeen Proving Ground, MD 21005	2	Director Petrol & Fld Svc Dept US Army Quartermaster School Fort Lee, VA 23801
1	Commander Materiel Test Directorate Bldg 400 Aberdeen Proving Ground, MD 21005	1	Commander US Army Electronics Research and Development Command ATTN: DRSEL-GG-TD Fort Monmouth, NJ 07703
1	Commander Edgewood Arsenal ATTN: SAREA-TS-L Aberdeen Proving Ground, MD 21010	1	President US Army Aviation Test Board ATTN: STEBG-MT Fort Rucker, AL 36360
1	Commander US Army Aberdeen Proving Ground ATTN: STEAP-TL Aberdeen Proving Ground, MD 21005	1	US Army Aviation School Library PO Drawer 0 Fort Rucker, AL 36360
1	Director US Army Materiel Systems Analysis Agency ATTN: DRXSY-CM Aberdeen Proving Ground, MD 21005	1	Commander Special Forces Detachment (Airborne), Europe APO New York 09050
1	Director US Army Engineer Waterways Experiment Station ATTN: Chief, Library Branch Technical Information Center Vicksburg, MS 39180	1	HQ, USAREUR & Seventh Army DCSENGR, ATTN: AEAEN-MO ATTN: Mil Ops Div APO New York 09403
1	Commander Picatinny Arsenal ATTN: SARPA-TS-S No. 59 Dover, NJ 07801	2	Engineer Representative US Army Standardization Group, UK Box 65, FPO New York 09510
		1	Commander Rock Island Arsenal ATTN: SARRI-LPL Rock Island, IL 61201

No. Copies	Addressee	No. Copies	Addressee
1	HQ, DA, ODCSLOG Directorate for Transportation and Services Army Energy Office Room 1D570 Washington, DC 20310	1	Commander Anniston Army Depot ATTN: Chemical Laboratory Anniston, AL 36202
1	Plastics Technical Evaluation Center Picatinny Arsenal, Bldg 176 ATTN: A. M. Anzalone SARPA-FR-M-D Dover, NJ 07801	2	Commander US Army General Materials & Petroleum Activity ATTN: STSGP-F STSGP-PE New Cumberland Army Depot New Cumberland, PA 17070
2	Commander Frankford Arsenal ATTN: Library, K2400, B1 51-2 SARFA-PDC Philadelphia, PA 19137	1	Commander US Army General Materials & Petroleum Activity ATTN: STSGP-PW Sharpe Army Depot Lathrop, CA 95330
1	Learning Resources Center US Army Engineer School Bldg 270 Fort Belvoir, VA 22060	1	Commander US Army Chemical Research & Development Laboratories ATTN: Directorate of Weapons Systems (SMUCR-WS) Edgewood Arsenal Aberdeen Proving Ground, MD 21010
1	President US Army Airborne, Communications & Electronics ATTN: STEBF-MA-A Fort Bragg, NC 28307	1	Commander US Army Arctic Test Activity APO 731 Seattle, WA 98731
2	Commander Headquarters, 39th Engineer Battalion (Cbt) Fort Devens, MA 01433	1	Commander US Army Alaska Support Command ATTN: ARCL-Q APO Seattle, WA 98749
1	President US Army Armor and Engineer Board ATTN: STEBB-TD-E Fort Knox, KY 40121	1	Commander US Army Materiel Maintenance Agency ATTN: AEZMPT-Q APO New York 09052
1	Commandant US Army Command and General Staff College ATTN: ATSCS-SE-L Fort Leavenworth, KS 66027	1	Director, Special Forces School US Army Inst for Military Assist ATTN: Training Division Fort Bragg, NC 28307
1	Commander 2nd Engineer Group ATTN: S4 APO San Francisco 96301	1	Commander US Army Aeronautical Depot Maintenance Center Naval Air Station ATTN: AMSAC-Q Corpus Christi, TX 78419

No. Copies	Addressee	No. Copies	Addressee
1	Commander US Army Foreign Science & Technology Center Federal Bldg ATTN: AMXST-GE Charlottesville, VA 22901	1	Information Ofc
1	Commander White Sands Missile Range ATTN: ORDBS-OM-Electro- Mechanical Labs	1	Legal Ofc
1	STEWS-LG-EC White Sands, NM 88002		Department of the Navy
3	Commander US Army Environmental Hygiene Agency Bldg 2400 Aberdeen Proving Ground, MD 21010	1	Director, Physics Program (421) Office of Naval Research Arlington, VA 22217
	USAMERADCOM	3	Director Naval Research Laboratory ATTN: Code 2627 Code 6200 Code 6180 Washington, DC 20375
1	Commander Technical Director Assoc Tech Dir/R&D Assoc Tech Dir/Engr & Acq Assoc Tech Dir/Matl Asmt Assoc Tech Dir/Tech Asmt CIRCULATE	1	Commander, Naval Facilities Engineering Command Department of the Navy ATTN: Code 10332 Washington, DC 20390
1	Chief, Lab 1000 Chief, Lab 2000 Chief, Lab 3000 Chief, Lab 4000 Chief, Lab 5000 Chief, Lab 6000 Chief, Lab 7000 Chief, Lab 8000 Chief, Lab 9000 Chief, TARSO CIRCULATE	1	US Naval Oceanographic Office Library (Code 1600) Washington, DC 20373
10	Fuels & Lubs Div	1	Officer-in-Charge (Code L31) Civil Engineering Laboratory Naval Construction Battalion Center Port Huenceme, CA 93043
10	M. Kolobielski	1	Director Earth Physics Program Code 463 Office of Naval Research Arlington, VA 22217
3	Tech Reports Ofc	1	Commandant US Marine Corps ATTN: Code AX Code A04H Washington, DC 20380
3	Security Ofc	1	Naval Ship Engineering Center Department of the Navy ATTN: SEC 6101E Washington, DC 20360
2	Tech Library	1	Commander Naval Ship Engineering Center Code 6101F Center Bldg Prince George's Center Hyattsville, MD 20782
1	Requirements & Programs Ofc		

No. Copies	Addressee	No. Copies	Addressee
2	Commander Naval Ordnance Systems Command ATTN: Technical Library (ORD-9132) Washington, DC 20360		Others
1	Commander US Naval Air Station Overhaul & Repair Department North Island San Diego, CA 92135	1	Professor Raymond R. Fox School of Engineering and Applied Science The George Washington University Washington, DC 20052
1	Superintendent US Naval Post Graduate School ATTN: Technical Reports Section Monterey, CA 93940	1	Chief, Marine & Earth Sciences Library NOAA, US Department of Commerce Rockville, MD 20852
1	Commander Naval Ship R&D Center Annapolis Laboratory ATTN: Technical Library Annapolis, MD 21402	1	Architectural and Engineering Development Information Center for Civil Defense 540 Engineering Building University of Florida Gainesville, FL 32601
	Department of the Air Force		
1	HQ USAF/RDPS (Mr. Allan Eaffy) Washington, DC 20330		
1	Mr. William J. Engle Chief, Utilities Branch HQ USAF/PREEU Washington, DC 20332		
1	AFSC/INJ Andrews AFB, MD 20334		
1	AFCEC/XR/21 Tyndall AFB, FL 32401		
1	HQ USAF/PREES ATTN: Mr. Edwin B. Mixon Bolling AFB-Bldg 626 Washington, DC 20332		
3	Commander Air Force Weapons Laboratory ATTN: AFWL-DEE		
1	AFWL-DEZ-S Air Force Systems Command Kirtland Air Force Base, NM 87117		