

UNCLASSIFIED

AD NUMBER

ADB017318

LIMITATION CHANGES

TO:

Approved for public release; distribution is unlimited.

FROM:

Distribution authorized to U.S. Gov't. agencies only; Test and Evaluation; DEC 1976. Other requests shall be referred to Air Force Weapons Laboratory, Attn: DED, Kirtland Air Force Base, NM 87117.

AUTHORITY

AFWL ltr, 29 Apr 1985

THIS PAGE IS UNCLASSIFIED

AD B017318

AUTHORITY: AFWL 17, 29 APR 85



AFWL-TR-76-65

AFWL-TR-76-65

2

AD B017318



DEVELOPMENT OF PIEZORESISTIVE BAR GAGE

CERF, University of New Mexico
Box 25, University Station
Albuquerque, NM 87131

December 1976

Final Report

Distribution limited to US Government agencies only because of test and evaluation of military systems/equipment (Dec 1976). Other requests for this document must be referred to AFWL(DED), Kirtland Air Force Base, New Mexico 87117.

This research was sponsored by the Defense Nuclear Agency under Subtask L11CAXSX352, Work Unit 55, Airblast Pressure Transducer Evaluation.

Prepared for
Director
DEFENSE NUCLEAR AGENCY
Washington, DC 20305

AIR FORCE WEAPONS LABORATORY
Air Force Systems Command
Kirtland Air Force Base, NM 87117

DDC
RECEIVED
APR 4 1977
RESERVED

A

DDC FILE COPY

This final report was prepared by the Eric H. Wang Civil Engineering Research Facility, University of New Mexico, Albuquerque, New Mexico, under Contract F29601-76-C-0015, Job Order WDNS0308, with the Air Force Weapons Laboratory, Kirtland Air Force Base, New Mexico. Mr. Santos J. Ayala (DED) was the Laboratory Project Officer-in-Charge.

When US Government drawings, specifications, or other data are used for any purpose other than a definitely related Government procurement operation, the Government thereby incurs no responsibility nor any obligation whatsoever, and the fact that the Government may have formulated, furnished or in any way supplied the said drawings, specifications, or other data, is not to be regarded by implication or otherwise, as in any manner licensing the holder or any other person or corporation, or conveying any rights or permission to manufacture, use, or sell any patented invention that may in any way be related thereto.

This technical report has been reviewed and is approved for publication.

Santos J. Ayala
SANTOS J. AYALA
Project Officer

Rudolph V. Matalucci
RUDOLPH V. MATALUCCI
Lt Colonel, USAF
Chief, Developmental Branch

Frank J. Leech
FRANK J. LEECH
Lt Colonel, USAF
Chief, Civil Engineering Research
Facility

DO NOT RETURN THIS COPY. RETAIN OR DESTROY.



UNCLASSIFIED

SECURITY CLASSIFICATION OF THIS PAGE (When Data Entered)

REPORT DOCUMENTATION PAGE		READ INSTRUCTIONS BEFORE COMPLETING FORM	
18. REPORT NUMBER AFWL-TR-76-65 ✓	2. GOVT ACCESSION NO.	3. RECIPIENT'S CATALOG NUMBER	
6. TITLE (and Subtitle) DEVELOPMENT OF PIEZORESISTIVE BAR GAGE.	9.	5. TYPE OF REPORT & PERIOD COVERED Final Report,	
7. AUTHOR(s) Kenneth B./Simmons	14.	5. PERFORMING ORG. REPORT NUMBER CERF-F1-4 ✓	
	15.	6. CONTRACT OR GRANT NUMBER(s) F29601-76-C-0015 ✓	
9. PERFORMING ORGANIZATION NAME AND ADDRESS Eric H. Wang Civil Engineering Research Facility University of New Mexico, Box 25, Univ Sta Albuquerque, NM 87131		10. PROGRAM ELEMENT, PROJECT, TASK AREA & WORK UNIT NUMBERS 62710H WDNS0308	
11. CONTROLLING OFFICE NAME AND ADDRESS Air Force Weapons Laboratory (DED) Kirtland Air Force Base, NM 87117		12. REPORT DATE December 1976	
14. MONITORING AGENCY NAME & ADDRESS (if different from Controlling Office) Director Defense Nuclear Agency Washington, D.C. 20305		13. NUMBER OF PAGES 34	
		15. SECURITY CLASS. (of this report) UNCLASSIFIED	
		15a. DECLASSIFICATION/DOWNGRADING SCHEDULE	
16. DISTRIBUTION STATEMENT (of this Report) Distribution limited to US Government agencies only because of test and evaluation of military systems/equipment (Dec 1976). Other requests for this document must be referred to AFWL (DED), Kirtland AFB, NM 87117.			
17. DISTRIBUTION STATEMENT (of the abstract entered in Block 20, if different from Report)			
18. SUPPLEMENTARY NOTES This research was sponsored by the Defense Nuclear Agency under Subtask L11CAXSX352, Work Unit 55, Airblast Pressure Transducer Evaluation.			
19. KEY WORDS (Continue on reverse side if necessary and identify by block number) Piezoresistive pressure bar gage Blast pressure measurement Instrumentation development			
20. ABSTRACT (Continue on reverse side if necessary and identify by block number) This report describes the adaptation of pressure bar techniques for pressure measurement to the development of a more reliable, useable, and rugged pressure gage for measuring pressure (up to 10,000 psi) in blast chambers and shock tubes. The pressure bar gage, used for years as a piezoelectric transducer, was converted to a piezoresistive transducer for easier use in field tests. Preliminary evaluation tests in the laboratory indicate that this gage combines the good dynamic response of damped pressure \approx (over)			

DD FORM 1 JAN 73 1473

EDITION OF 1 NOV 65 IS OBSOLETE

UNCLASSIFIED

SECURITY CLASSIFICATION OF THIS PAGE (When Data Entered)

400 976

LB

UNCLASSIFIED

SECURITY CLASSIFICATION OF THIS PAGE(When Data Entered)

ABSTRACT (cont'd)

bar gages (fast rise time with little overshoot and ringing) with the static response capabilities and reliability of the more common diaphragm pressure gages. Initial use in a field test indicated that the gage can survive high-velocity debris impact, although usually with some zero offset. This offset can probably be eliminated by using soft debris shields.

UNCLASSIFIED

SECURITY CLASSIFICATION OF THIS PAGE(When Data Entered)

CONTENTS

<u>Section</u>		<u>Page</u>
I	INTRODUCTION	3
II	PIEZORESISTIVE BAR GAGE DEVELOPMENT	6
	Original Piezoresistive Bar Gage	6
	Redesigned Piezoresistive Bar Gage	12
III	PRESSURIZED BAR GAGE DEVELOPMENT	18
IV	DEVELOPMENT AND EVALUATION OF FIELD GAGE	21
V	CONCLUSIONS AND RECOMMENDATIONS	26

ACCESSION for	
NTIS	White Section <input checked="" type="checkbox"/>
DDC	Soft Section <input checked="" type="checkbox"/>
UNANNOUNCED	<input type="checkbox"/>
JUSTIFICATION.....	
BY.....	
DISTRIBUTION/AVAILABILITY CODES	
Dist.	AVAIL. OR/ SPECIAL
B	

ILLUSTRATIONS

<u>Figure</u>		<u>Page</u>
1	Piezoelectric Pressure Bar Gage (Model ST-4)	5
2	Original Piezoresistive Bar Gage	7
3	Original Piezoresistive Bar Gage Responses	8
4	Response of Original Piezoresistive Bar Gage to Pressure Step	9
5	Original Piezoresistive Bar Gage with Pressure Relief Ring	10
6	Response of Original Piezoresistive Bar Gage with Pressure Relief Ring to Pressure Step	10
7	High-Pressure Results of Original Piezoresistive Bar Gage	11
8	Redesigned Piezoresistive Bar Gage	13
9	Test Results of Redesigned Piezoresistive Bar Gage	14
10	Test Setup for Cross-Axis Acceleration Tests	16
11	Typical Data from Cross-Axis Acceleration Tests of Redesigned Piezoresistive Bar Gage	16
12	Typical Error Signal Versus Acceleration Level for Redesigned Piezoresistive Bar Gage	17
13	Pressurized Piezoresistive Bar Gage	19
14	Redesigned Piezoresistive Bar Gage Modified for Extrusion-Filling Process	22
15	Filling Fixture for Extrusion-Filling Process	23
16	Shock-Tube Results of Extrusion-Filled Redesigned Piezoresistive Bar Gage	24
17	Shock-Tube Calibration of Redesigned Piezoresistive Bar Gage	25

SECTION I INTRODUCTION

BACKGROUND

Blast-effect simulation of nuclear weapons has generally been accomplished with explosive-filled chambers designed to generate specified blast pressures and durations. These simulations are generally conducted as disposable (i.e., one shot) field tests. Pressure pulses within these chambers are usually characterized by large pressure spikes, high temperatures, and large amounts of debris flying about the cavity. Measurement of pressure under these conditions is usually more difficult than that under cleaner environments, such as in a gas-driven shock tube. Usually, in the past, these measurements were accomplished with piezoresistive (i.e., strain gage) diaphragm-type pressure gages. However, these gages can be damaged by the large pressure spikes, which can cause diaphragm resonance and possible overranging of the gage, as well as by debris impact. Another class of pressure gage that could be used is the pressure bar gage. Since pressure bar gages are usually built as piezoelectric gages, their use in the field has been limited because of cable-noise problems. However, if the principle of pressure bar gage operation could be applied to explosive-chamber pressure measurements, significant improvements in pressure-data recovery might be realized.

Piezoelectric pressure bar gages were developed a number of years ago to measure pressures in gaseous detonation waves and in shock tubes. A small metal bar was used to transmit the pressure to a piezoelectric sensor. The metal bar and the piezoelectric sensor were acoustically matched to prevent reflections at the interface. (This was usually accomplished with aluminum bars and quartz disks.) In early versions, a backup bar of similar size and acoustic impedance was used to delay the reflection time from the end of the bar (ref. 1). This resulted in a gage with a relatively short recording time, depending on the length of the backup bar. The primary advantages of piezoelectric pressure bar gages are their very fast rise time and very little resonance.

1. Edwards, D. H., Journal of Scientific Instruments, Vol. 35, 1958, p. 346.

A significant improvement in piezoelectric pressure bar gages is reported in reference 2. In these gages a tapered backup bar encased in wax is used. The wax sheath acts to absorb the stress pulse transmitted into the backup bar and thus prevents unwanted reflections and greatly extends the recording time. It has been demonstrated both analytically and experimentally that if the piezoelectric crystal cannot be placed on the pressurized end of the bar (considered impractical because of sealing and bar support problems), the optimum crystal location is somewhere between two and four bar diameters from the input end (ref. 2). This crystal location is the best compromise between fast rise time and minimized ringing due to wave dispersion in the metal pressure bar.

A further development of the piezoelectric bar gage (fig. 1) was made at the Ballistics Research Laboratory (BRL) (ref. 3). This development overcame the sealing and bar support problems. The piezoelectric sensor is located on the input end of the pressure bar to achieve a very fast rise time. The pressure bar, which is acoustically matched to the sensor, is embedded in an absorptive material (a relatively hard epoxy) to dissipate the stress pulse into the surrounding material. The electrical circuit is completed by a thin silver plating between the exposed face of the sensor and the gage case. This gage (Model ST-4) is commercially available.* The ST-4 gage probably has the fastest rise time of any commercial pressure gage. If properly used, the ST-4 gage has a rise time of about 0.2 μ sec. It also has very little overshoot (less than about 10 percent) and essentially no resonance. It is, however, very temperature-sensitive because of the exposed piezoelectric sensor.

Because of piezoelectric circuitry problems in field tests and the temperature sensitivity of commercially available pressure bar gages, an effort was undertaken at the Civil Engineering Research Facility (CERF) several years ago to

2. Edwards, D. H.; Davis, L., and Lawrence, T. R.; "The Application of a Piezoelectric Bar Gage to Shock Tube Studies," Journal of Scientific Instruments, Vol. 41, 1964, pp. 609-613.
3. Granath, B. A., and Coulter, G. A., BRL Shock Tube Piezo-Electric Blast Gages, BRL Technical Note No. 1478, Aberdeen Proving Ground, Maryland, August 1962.

*Susquehanna Instruments Company, Rt. 2, Box 228, Havre de Grace, Maryland 21078.

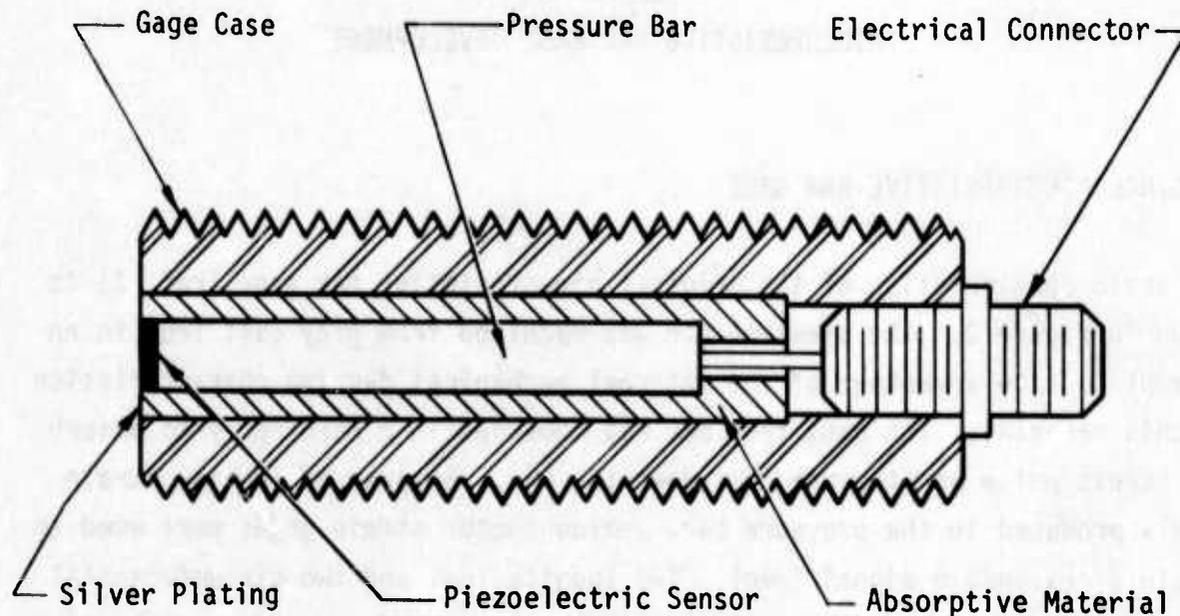


Figure 1. Piezoelectric Pressure Bar Gage (Model ST-4)

develop a piezoresistive bar gage. It became apparent that if the sensing elements were changed from piezoelectric to piezoresistive (i.e., strain gages) and placed a small distance from the end of the bar, both of these problems could be reduced, while retaining the advantages of pressure bar gages (fast rise time and low resonance). In addition, such a gage should be much less likely to be damaged by debris. Initial development work on a piezoresistive bar gage was described previously (ref. 4). That development is summarized in this report and subsequent developments at CERF are presented.

4. Crist, Robert A. and Simmons, Kenneth, Dynamic Economical Large Testing Apparatus--A Blast Pressure Loading Technique, AFWL-TR-71-151, Air Force Weapons Laboratory, Kirtland Air Force Base, New Mexico, June 1972.

SECTION II PIEZORESISTIVE BAR GAGE DEVELOPMENT

ORIGINAL PIEZORESISTIVE BAR GAGE

The basic configuration of the original piezoresistive bar gage (ref. 4) is shown in figure 2. The pressure bar was machined from gray cast iron in an attempt to take advantage of the internal mechanical damping characteristics of this material. The cast iron bar was embedded in a hard epoxy to absorb the stress pulse as it propagates down the bar. Because of the low strain levels produced in the pressure bar, semiconductor strain gages were used to obtain a reasonable signal level. Two longitudinal and two circumferential gages were mounted on the bar close to the pressurized end and connected into a full bridge for temperature compensation.

Results of preliminary evaluation tests on the original piezoresistive bar gage are shown in figure 3. The tests were conducted in a 2-in-diameter, air-driven shock tube with the gages mounted end-on in the tube to measure reflected pressure. A reflected pressure of about 250 psi was used. The upper trace in each record is from the piezoresistive bar gage and the lower one is from an ST-4 gage. The first record (fig. 3a) shows that the piezoresistive bar gage maintained most of the fast rise time associated with pressure bar gages. Both gages show a rise time of about 2 μ sec. The second record (fig. 3b), at a slower sweep rate, shows that the piezoresistive bar gage is much less temperature-sensitive than the ST-4 gage. As the shock wave reflected back and forth through the closed-end shock tube, the pressure built up to the static chamber pressure. The piezoresistive bar gage followed that static pressure reasonably well; whereas, the ST-4 gage began drifting fairly rapidly because of temperature sensitivity.

Tests of original piezoresistive bar gage models (fig. 2) involving long-duration pressure steps indicated drift problems after several seconds (fig. 4). It was suspected that the drift was due to creep within the epoxy potting compound used to encase the pressure bar. As the epoxy creeps it loads the side of the bar and reduces the longitudinal strain thus decreasing the



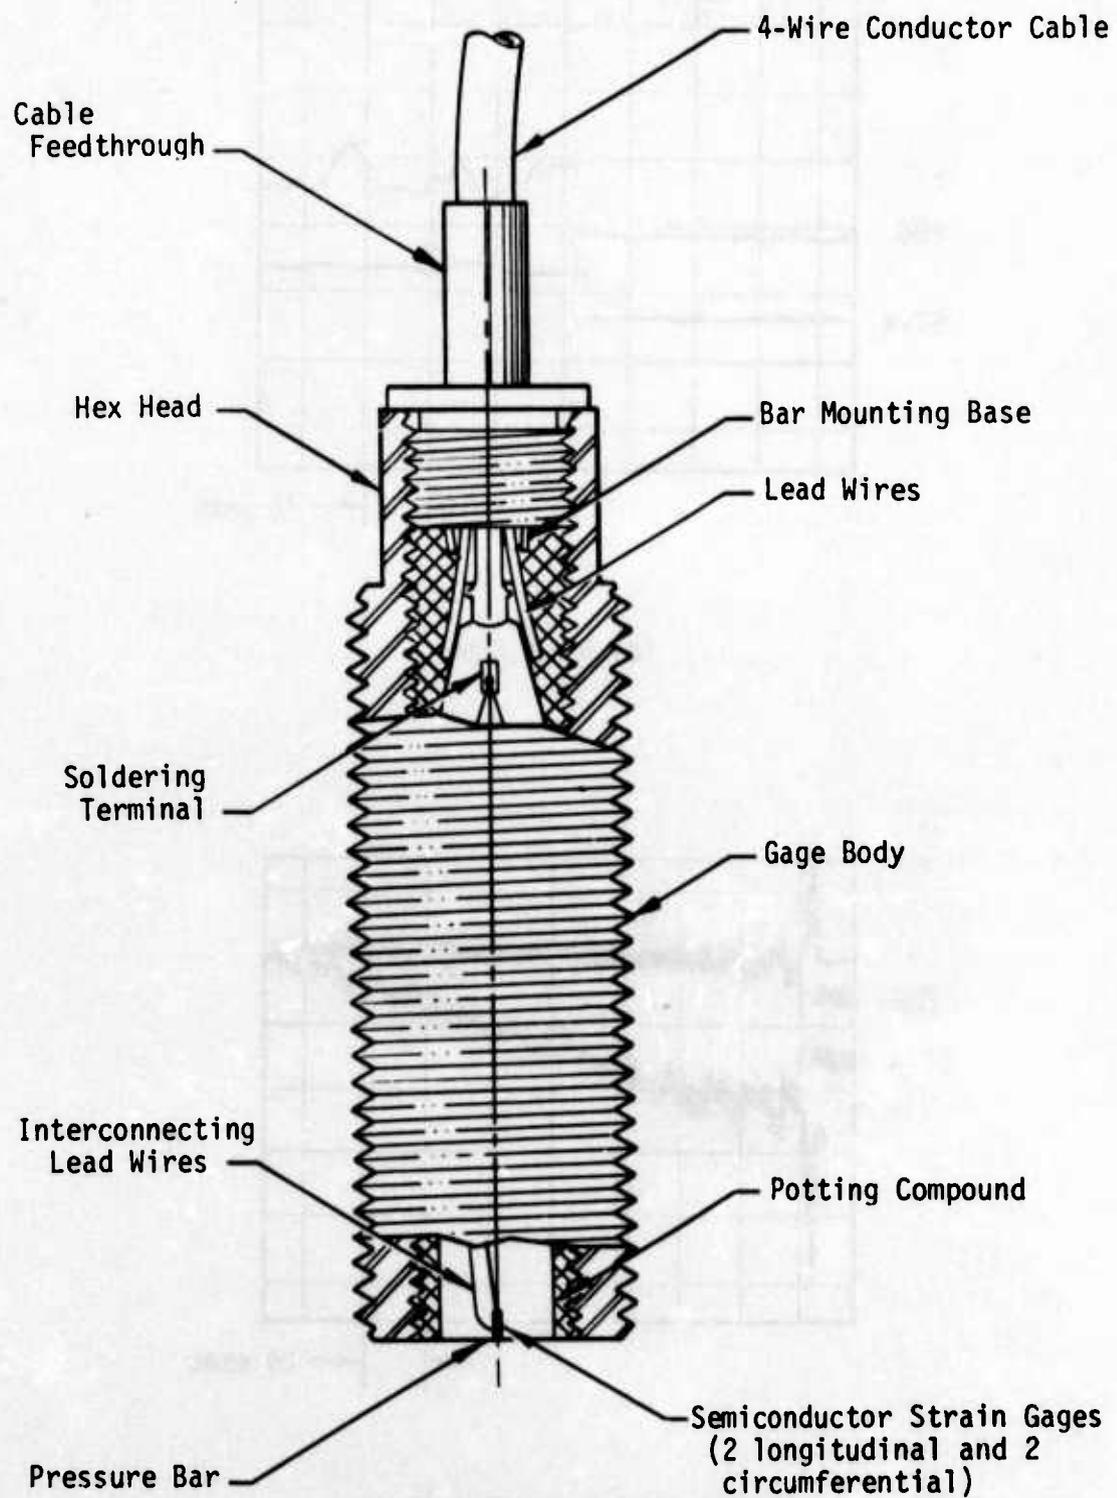


Figure 2. Original Piezoresistive Bar Gage

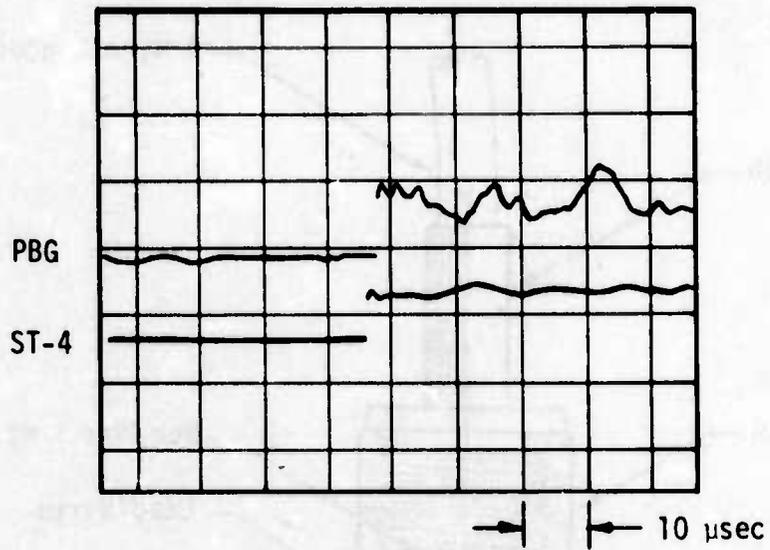

(a) Rise Time

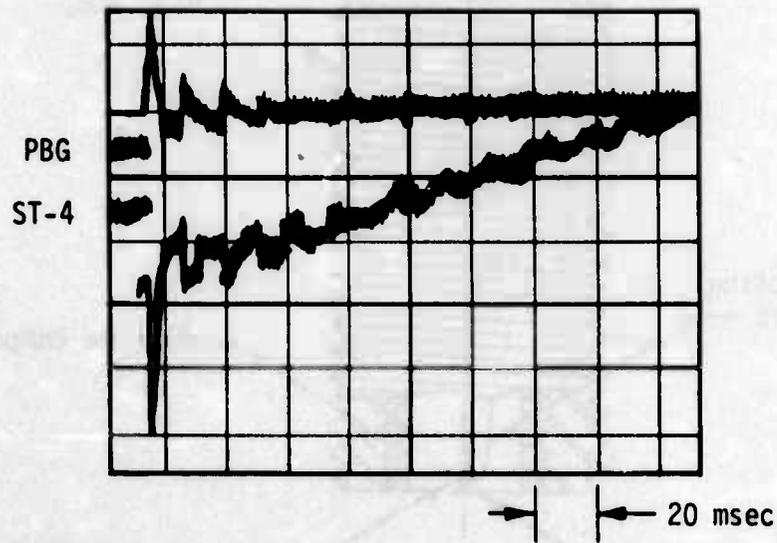

(b) Temperature Sensitivity

Figure 3. Original Piezoresistive Bar Gage Responses

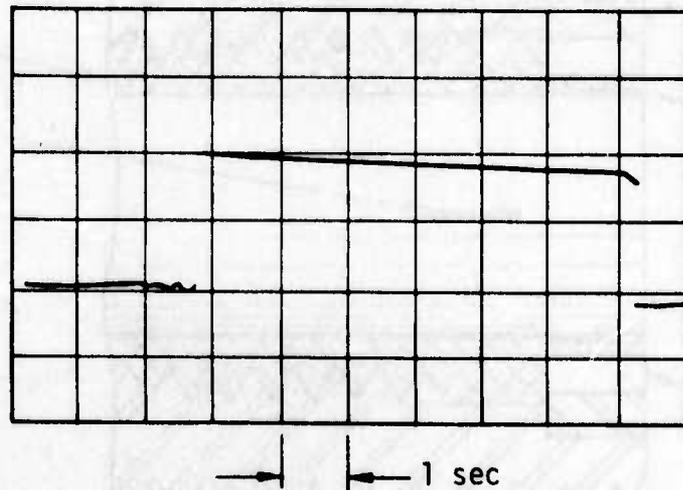


Figure 4. Response of Original Piezoresistive Bar Gage to Pressure Step

gage output. To eliminate this long-duration drift, a pressure relief ring (fig. 5) was installed in the end of the piezoresistive bar gage. This ring prevented the fluid pressure being measured from acting on the potting compound. A Teflon film was installed between the pressure relief ring and the pressure bar to reduce friction. The results of the pressure relief ring modification (fig. 6) indicates that the drift was essentially eliminated.

Both static and dynamic high-pressure tests on the piezoresistive bar gage are reported in reference 4. The static tests indicated very good linearity up to about 5,000 psi and less than 4 percent nonlinearity up to 10,000 psi (fig. 7a). The dynamic test results (fig. 7b) were obtained with a high-pressure helium/freon shock tube. The piezoresistive bar gage reproduced the ST-4 trace reasonably well, with respect to both amplitude and waveform.

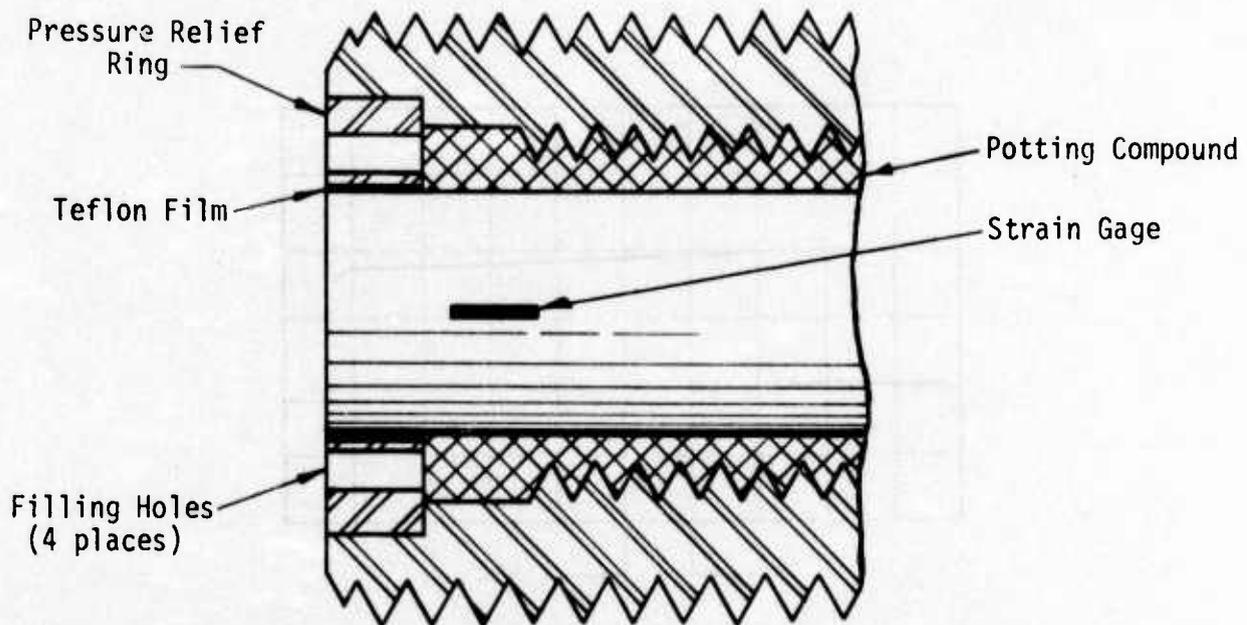


Figure 5. Original Piezoresistive Bar Gage with Pressure Relief Ring



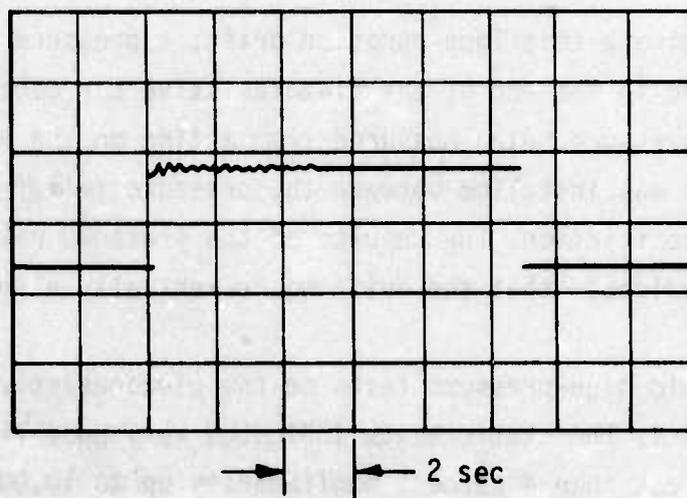


Figure 6. Response of Original Piezoresistive Bar Gage with Pressure Relief Ring to Pressure Step

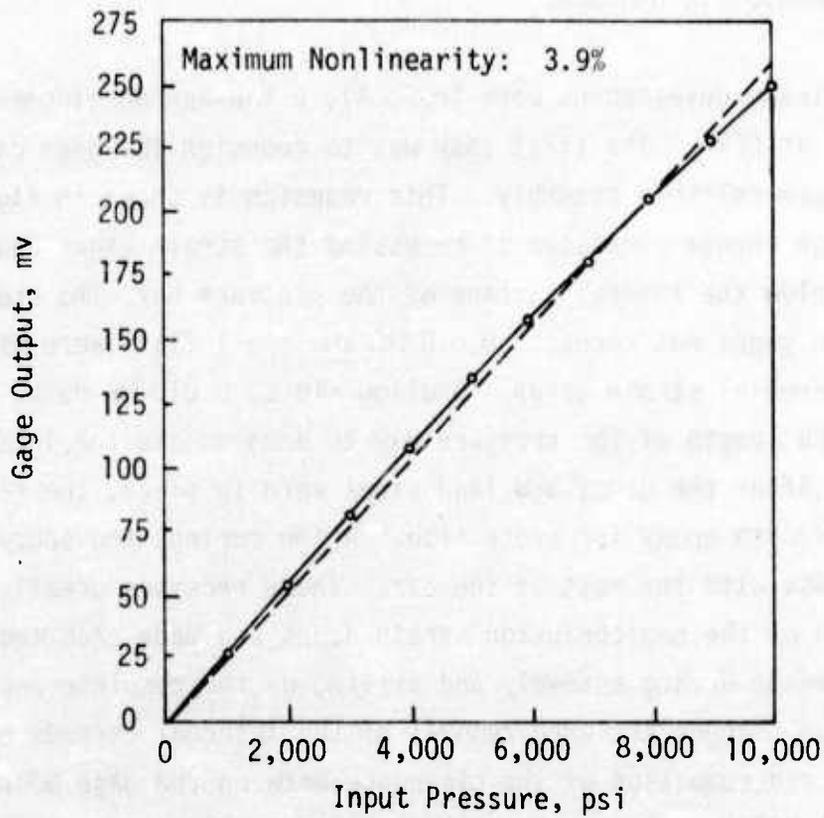

(a) Static Response

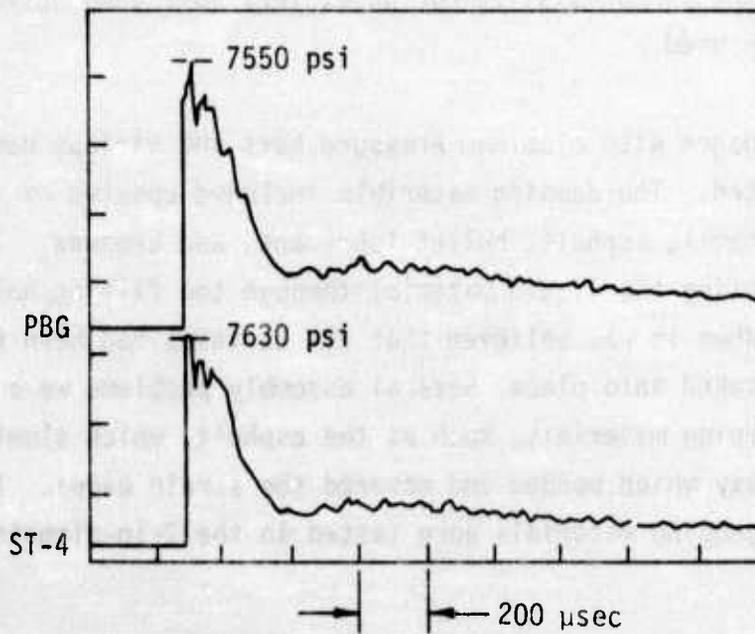

(b) Dynamic Responses

Figure 7. High-Pressure Results of Original Piezoresistive Bar Gage

REDESIGNED PIEZORESISTIVE BAR GAGE

After the preliminary development work (ref. 4), a low-key developmental effort continued at CERF. The first task was to redesign the gage case for easier and more reliable assembly. This redesign is shown in figure 8. The primary design change consisted of recessing the strain gages and lead wires slightly below the lateral surface of the pressure bar. The area around the strain gages was recessed 0.010 in. and small flats were machined for the circumferential strain gages. Shallow slots, 0.010 in. deep, were machined along the length of the pressure bar to accommodate the interconnecting lead wires. After the gages and lead wires were in place, the recessed areas were potted with epoxy for protection. After curing, the epoxy was machined down flush with the rest of the bar. These recesses greatly facilitated application of the semiconductor strain gages and made them much less susceptible to damage during assembly and filling of the complete pressure gage. Other design changes included removal of the internal threads next to the pressure bar and reduction of the clearance between the gage body and the pressure bar to 0.008 in. Also, the filling holes in the pressure relief ring were sealed with brass pins, which were staked into place. By completely sealing the end of the piezoresistive bar gage, very soft damping materials such as wax could be used.

Piezoresistive bar gages with aluminum pressure bars and various damping materials were constructed. The damping materials included epoxies of various hardnesses, Wood's metal, asphalt, bullet lubricant, and beeswax. The gages were filled by injecting the liquid material through the filling holes in the front of the gage. When it was believed that all cavities had been filled, the sealing pins were staked into place. Several assembly problems were encountered with some of the damping materials, such as the asphalt, which slowly attacked and softened the epoxy which bonded and covered the strain gages. The gages with these various damping materials were tested in the 2-in-diameter, air-driven shock tube.

The results of the tests generally indicated that the beeswax was the best damping material. Results of tests with soft epoxy and beeswax are compared in figure 9. The soft epoxy allowed considerable ringing in the gage (fig. 9a); the beeswax essentially damped out all of this ringing (fig. 9b). However,



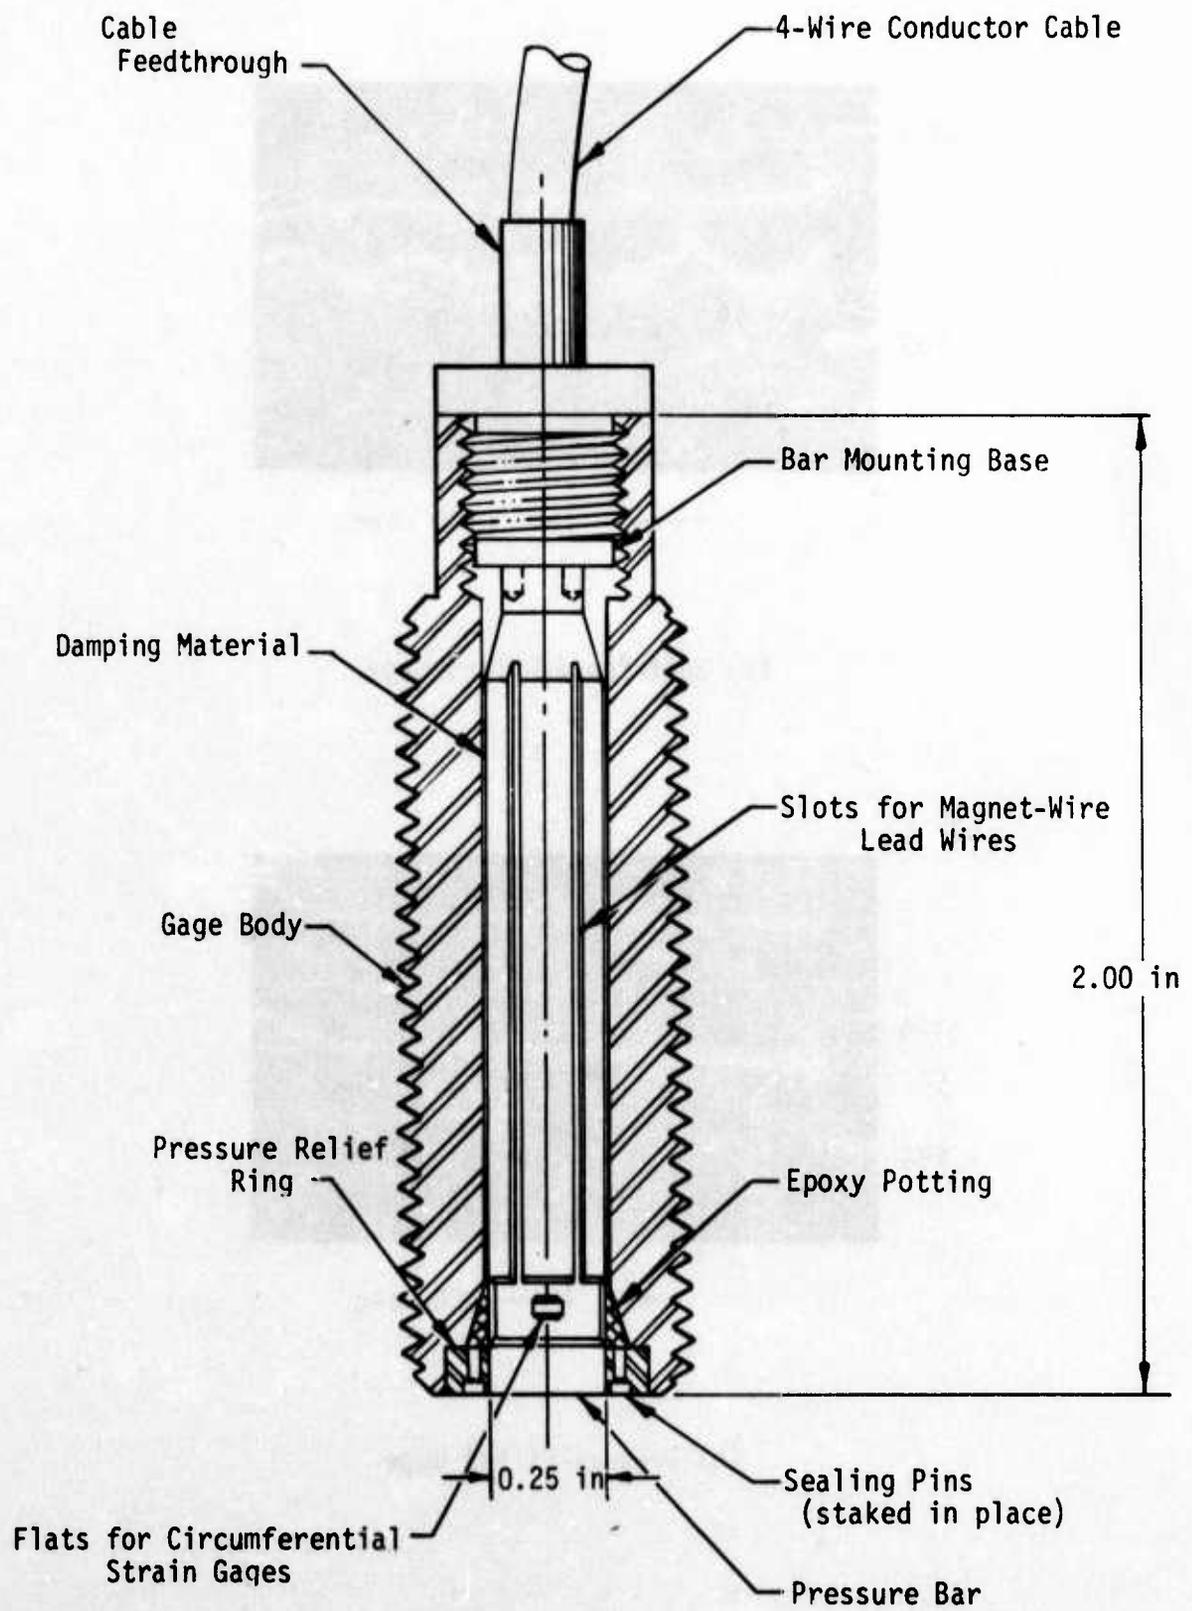


Figure 8. Redesigned Piezoresistive Bar Gage

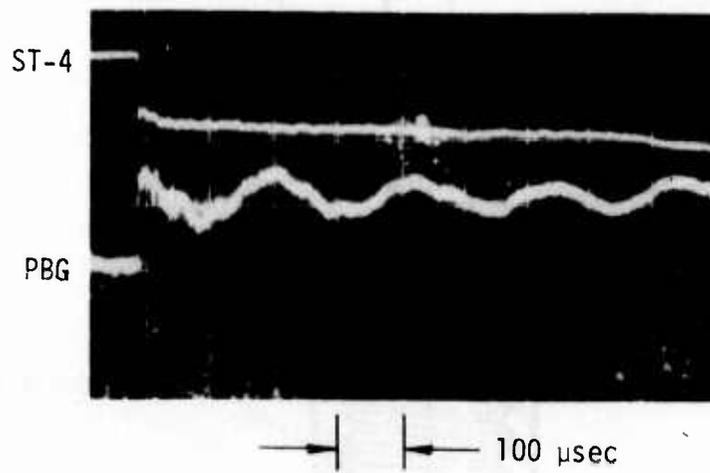

(a) Soft-Epoxy-Filled Gage

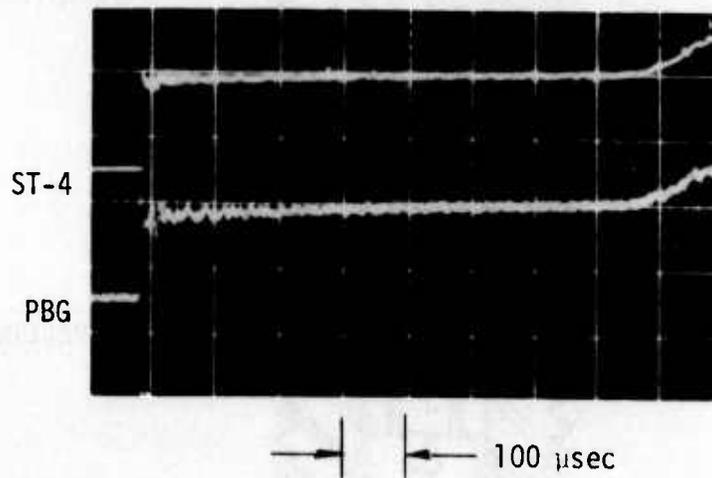

(b) Beeswax-Filled Gage

Figure 9. Test Results of Redesigned Piezoresistive Bar Gage

it was often difficult to get the beeswax into the gage well enough to produce the damping shown in figure 9b. Also, once in and sealed, the beeswax would apparently separate from the pressure bar and damping would be reduced. This separation, which would sometimes take several weeks to occur, was probably caused by cavities inadvertently left within the beeswax and by the high coefficient of thermal expansion of beeswax.

Since the piezoresistive bar gage was suspected of being sensitive to cross-axis acceleration, acceleration-sensitivity tests were conducted on several well-damped, beeswax-filled gages. The test setup consisted of a steel Hopkinson pressure bar loaded by a short steel striker bar (fig. 10). The piezoresistive bar gage was mounted close to the free end in a hole drilled and tapped into the bar. Acceleration was measured by an accelerometer mounted on the free end of the Hopkinson bar. Each test usually consisted of a series of five or six loadings at various acceleration levels (controlled by the striker bar impact velocity).

Typical data from the tests are shown in figure 11. The top trace indicates the acceleration level; the bottom trace shows the acceleration-induced signal from the piezoresistive bar gage. The results of one of the test series are plotted in figure 12. This plot shows a distinct leveling off of the pressure gage output with increasing acceleration levels. For this particular gage, the transverse acceleration sensitivity (defined as pressure gage output divided by acceleration level) at 4300 g was 0.032 psi/g, based on a faired curve through the data points. This acceleration sensitivity value was fairly typical for all the beeswax-filled gages; and although it is fairly high when compared to that for certain types of diaphragm pressure gages, this value is not so high as to discourage further development. These relatively high values simply mean that in high-acceleration environments, it may be advisable to use some sort of mechanical noise isolation when mounting the piezoresistive bar gage.

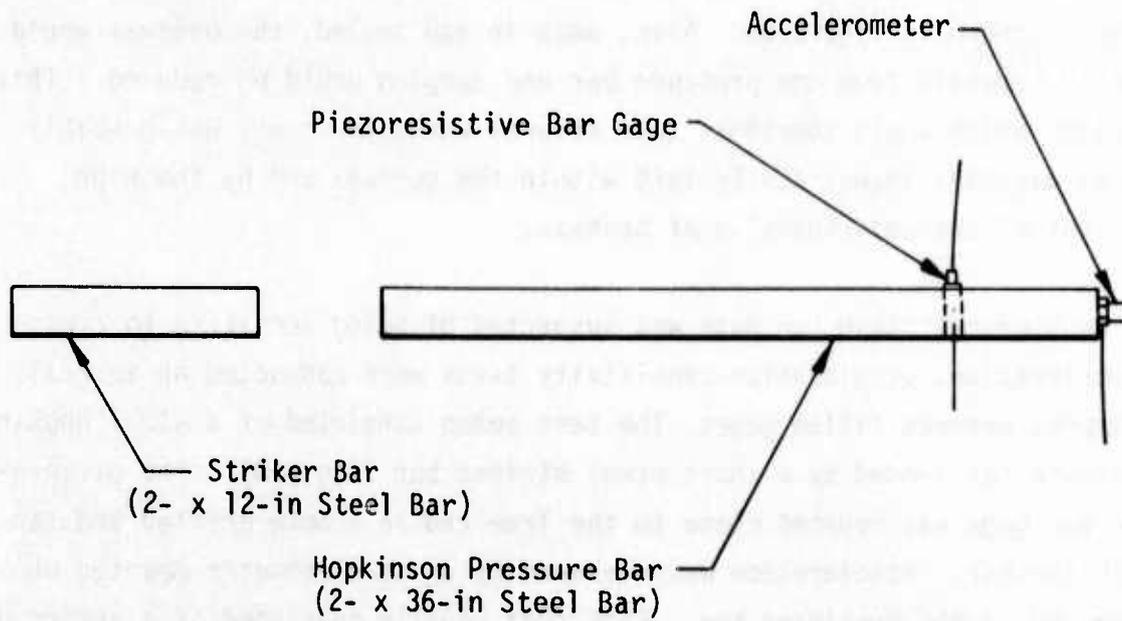


Figure 10. Test Setup for Cross-Axis Acceleration Tests

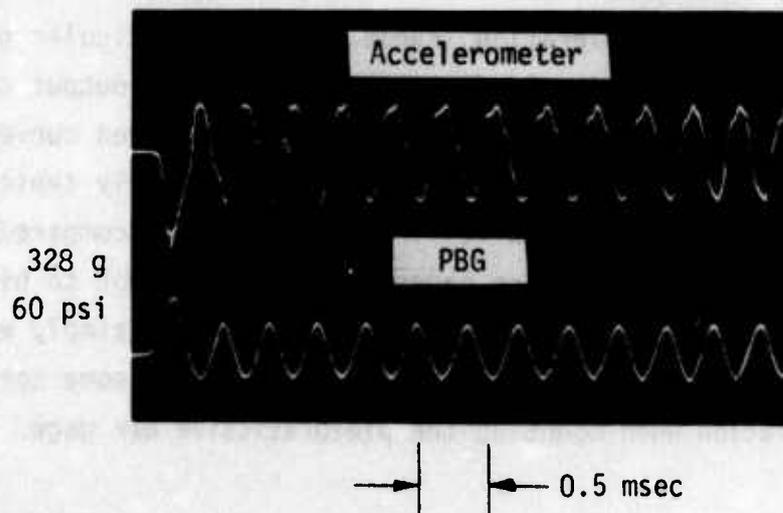


Figure 11. Typical Data from Cross-Axis Acceleration Tests of Redesigned Piezoresistive Bar Gage

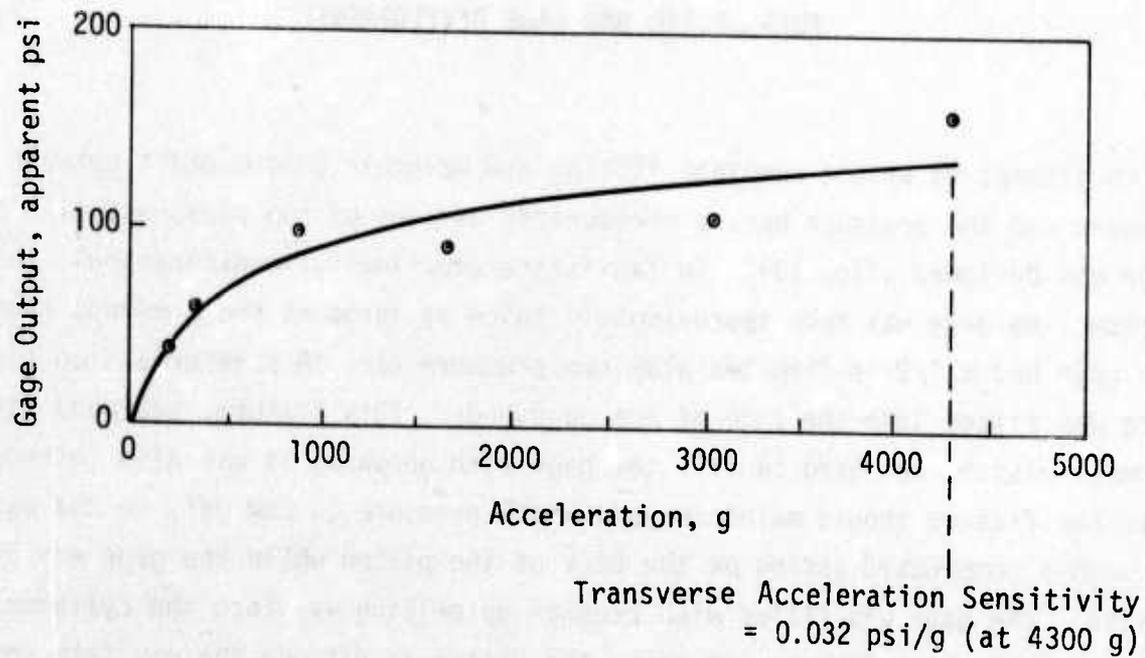


Figure 12. Typical Error Signal Versus Acceleration Level for Redesigned Piezoresistive Bar Gage

SECTION III

PRESSURIZED BAR GAGE DEVELOPMENT

In an attempt to assure complete filling and maintain good contact between the beeswax and the pressure bar, a pressurized version of the piezoresistive bar gage was designed (fig. 13). To facilitate experimental modifications, this pressurized gage was made approximately twice as large as the previous gages. The gage had a 1/2-in-diameter aluminum pressure bar. A pressurization fixture was fitted into the side of the gage body. This fixture, equipped with a small piston, was used to fill the gage with beeswax; it was also intended that the fixture should maintain some small pressure (a few psi) on the wax through a compressed spring on the back of the piston while the gage was being tested. The gage was filled with beeswax by melting wax into the cylinder of the pressurization fixture and using the piston to extrude the wax into the gage. The holes in the pressure relief ring on the front of the gage served as vents. Wax was extruded into the gage until continuous ribbons of wax came out all four vent holes, at which time the vent holes were sealed with small screws.

The first attempt to fill the pressurized gage resulted in the epoxy joint between the pressure bar and the bar mounting base being broken because of excessive extrusion pressure on the wax. The gage was disassembled and a new pressure bar was fabricated with the mounting base machined as an integral part of the pressure bar. The gage was reassembled and filling of the gage was accomplished with little difficulty.

The pressurized bar gage was first tested in an unpressurized mode in the 2-in-diameter, air-driven shock tube. The results indicated that good damping had been achieved by the extrusion-filling process. The gage was retested periodically for about a month with no apparent degradation of the damping characteristics. It then became apparent that if the gage was completely filled by the extrusion-filling process, continuous external pressurization of the wax during testing and use of the gage would be unnecessary.

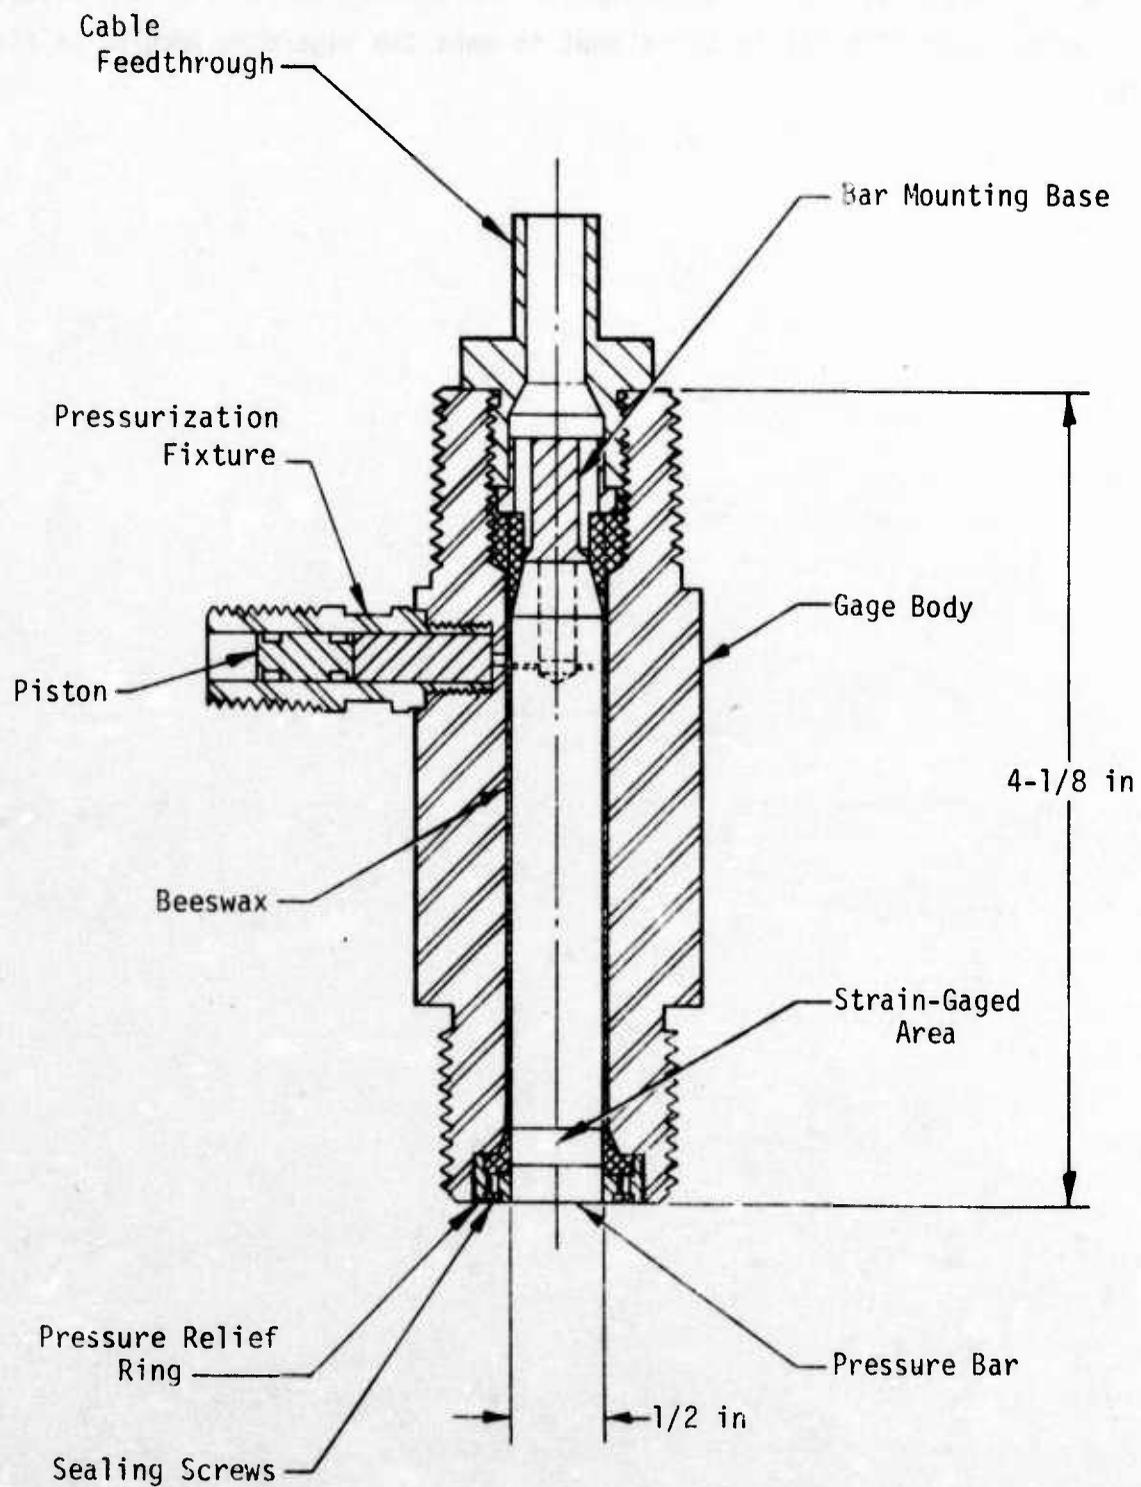


Figure 13. Pressurized Piezoresistive Bar Gage

With the apparent good results of the extrusion-filling process, the decision was made to apply this filling process to the smaller version of the piezoresistive bar gage (fig. 8) in an attempt to make the gage more usable in field tests.

SECTION IV
DEVELOPMENT AND EVALUATION OF FIELD GAGE

The gage shown in figure 8 (1/4-in-diameter pressure bar) was modified for use with the wax extrusion-filling process. The modified gage is shown in figure 14. A small filling hole was drilled in the side of the gage body toward the back end of the pressure bar. The external threads were removed from the gage body in this region to facilitate the fit into the filling fixture. The pressure bar and the mounting base were machined as an integral part, as with the pressurized gage.

The filling fixture for the extrusion-filling process consisted of a gage holder block, a filling cylinder with a small tip machined to fit the filling hole in the gage body, and a piston with a weight platform (fig. 15). The gage was placed in the holder block with the filling hole aligned with the centerline of the filling cylinder. The cylinder (previously filled with wax) was screwed down until the tip engaged the filling hole. Weights were then placed on the weight platform to slowly extrude the wax into the gage. A pressure of about 200 psi was maintained in the filling cylinder until the ribbons of wax coming through the vent holes were continuous and no air bubbles were evident. The gage was then removed and all vent holes were sealed with brass pins staked into place.

The extrusion-filled piezoresistive bar gages intended for field usage were subjected to a number of preliminary evaluation tests including tests in the 2-in-diameter, high-pressure, helium/freon shock tube. The results of the shock-tube tests showed that good damping was achieved (fig. 16a) and the fast rise time was preserved (fig. 16b).

Cross-axis acceleration sensitivity tests were conducted on one of the field gages. The result was essentially the same as that shown in figure 12. This indicates that acceleration sensitivity was neither increased nor decreased by the improved filling process.

Fourteen piezoresistive bar gages like the one shown in figure 14 were built for the Dynamic Air Blast Simulator (DABS) IA Project (a large expendable shock-tube type of field test). Eleven of the fourteen gages had hardened

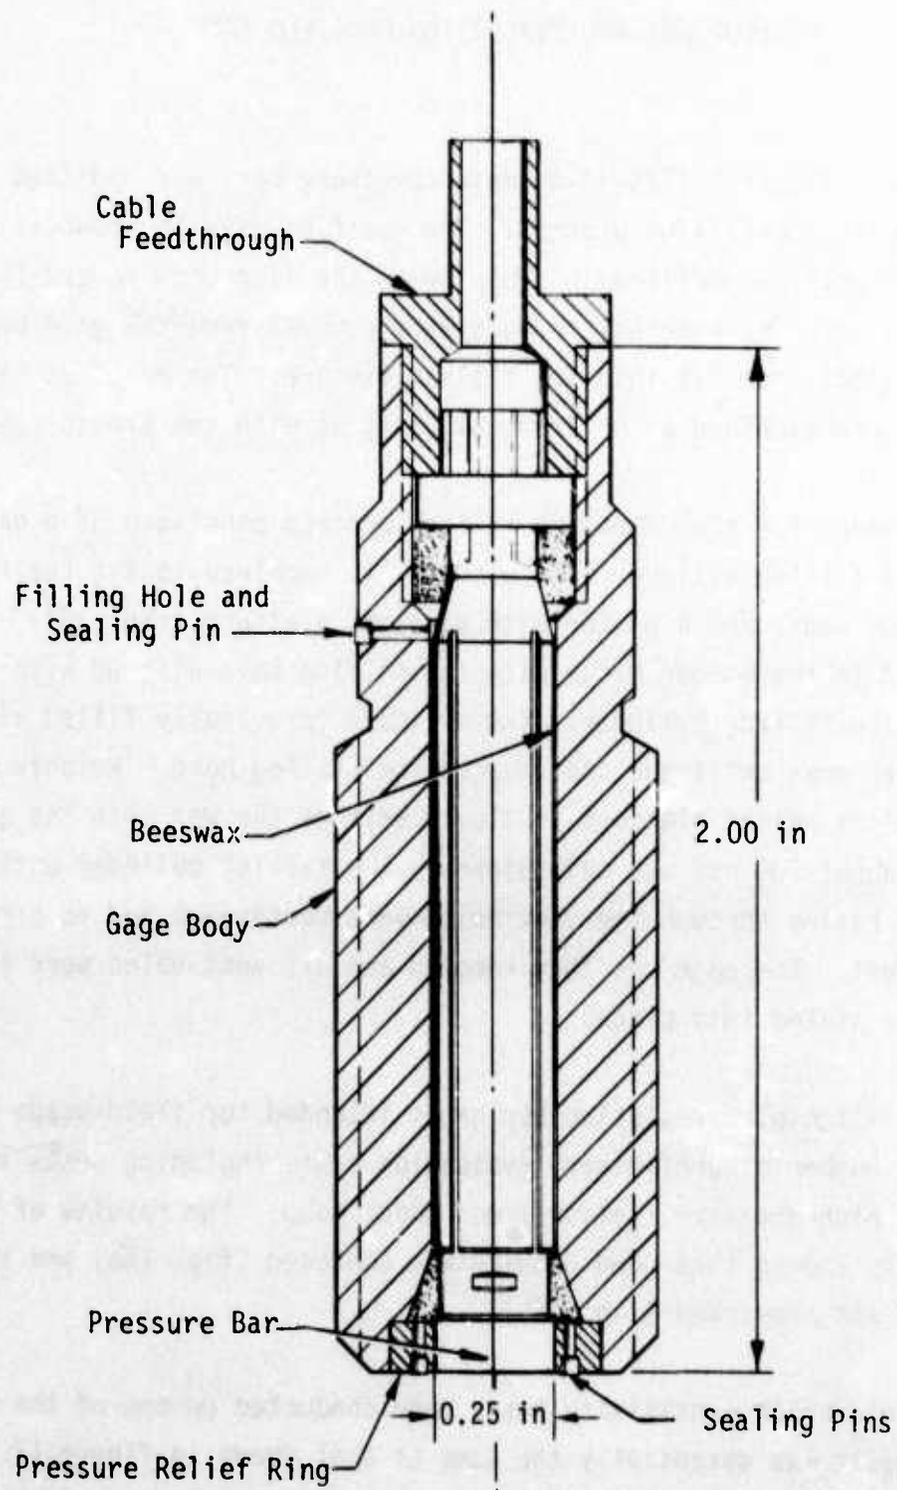


Figure 14. Redesigned Piezoresistive Bar Gage Modified for Extrusion-Filling Process



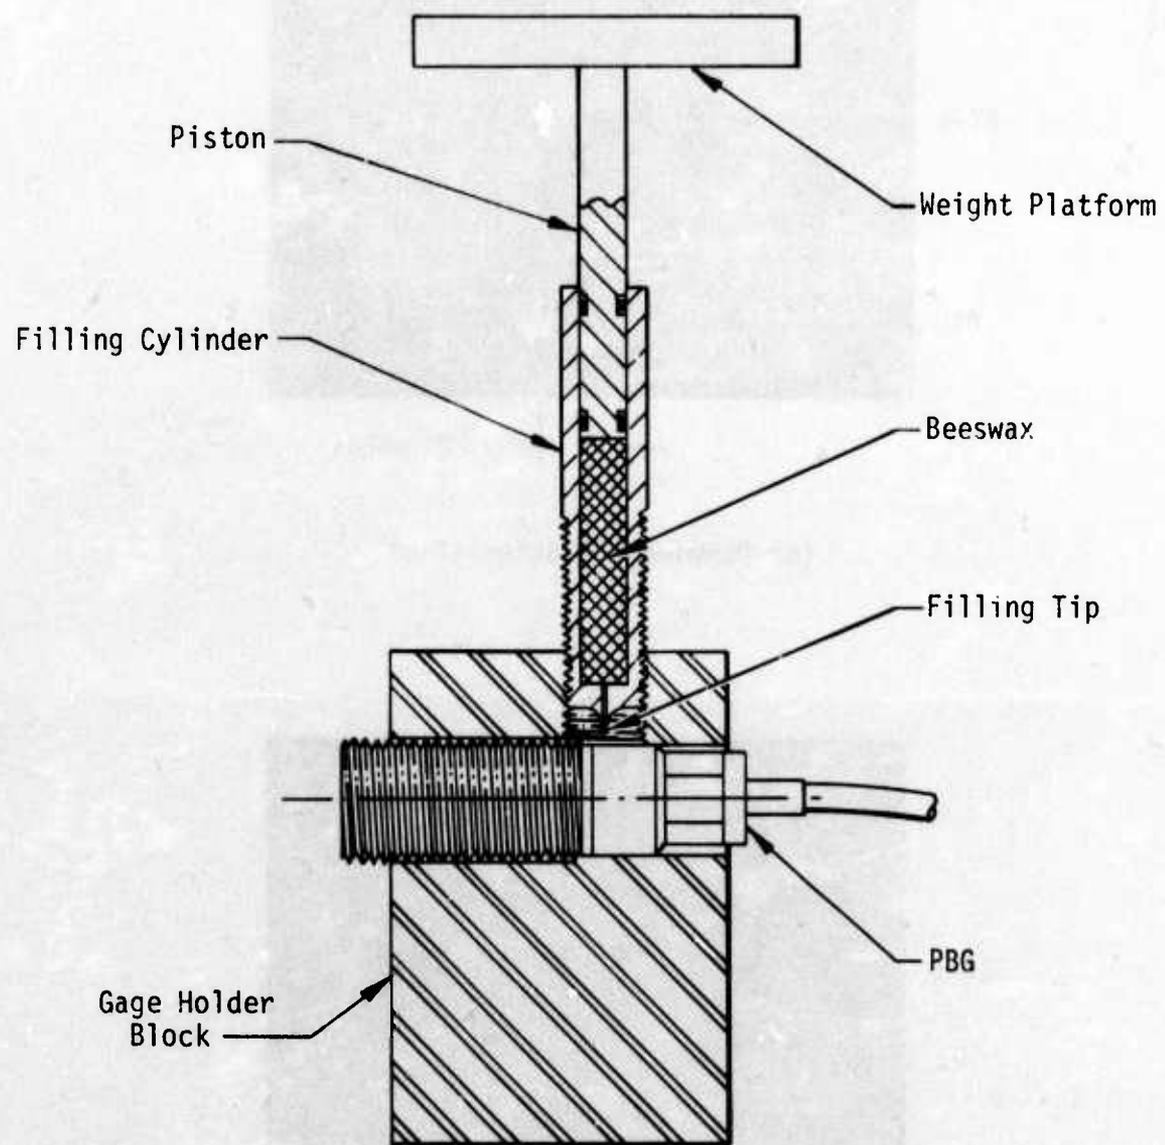


Figure 15. Filling Fixture for Extrusion-Filling Process

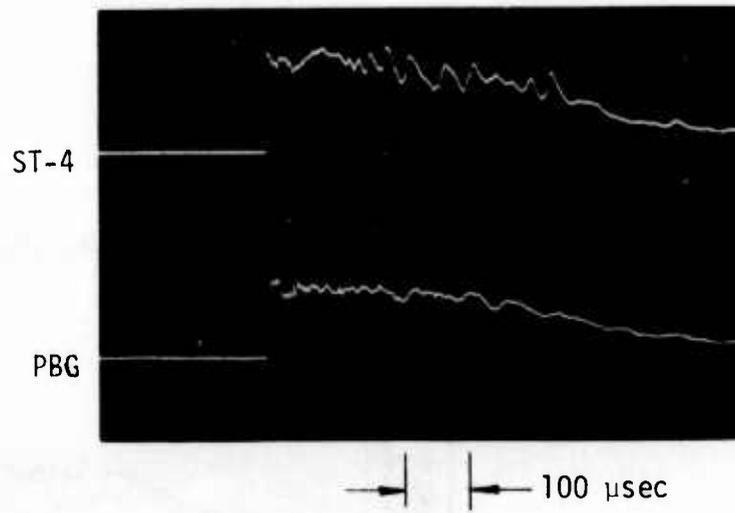

(a) Damping Characteristics

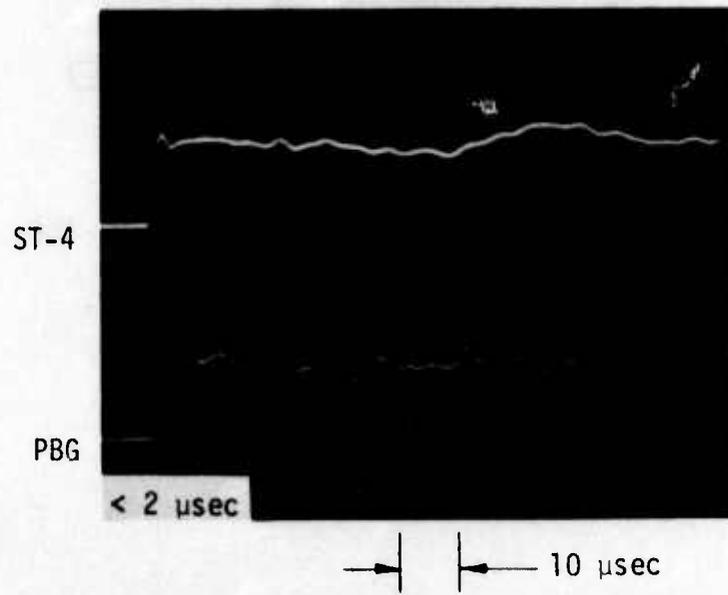

(b) Rise Time

Figure 16. Shock-Tube Results of Extrusion-Filled Redesigned Piezoresistive Bar Gage

steel pressure bars. This gave these gages an effective range of about 30,000 psi, with an overrange capability of about 100,000 psi. These higher-range gages were used because of the large pressure spikes and debris expected in the DABS IA Test.

The 14 gages were dynamically calibrated in the 2-in-diameter, high-pressure shock tube with an ST-4 gage as a reference. These calibrations were conducted at three different pressure levels (approximately 500, 1500, and 3000 psi). The result of one of these calibrations is shown in figure 17. This plot indicates reasonable dynamic linearity up to about 3000 psi.

The 14 gages were used in the DABS IA Test with reasonable success. Nine of the gages were placed in stagnation probes where they were subjected to particle impacts at about 5000 ft/sec and stagnation pressures of about 3000 psi. Six of the nine stagnation gages continued to read after debris impact, although sometimes with significant zero offsets. The zero offsets were probably caused by impact-generated inelastic deformation within the steel bar. It may be possible to reduce this offset by shielding the pressure bar with a softer material, such as lead. A soft shield should help to reduce the impact-generated stress levels before they are propagated into the steel pressure bar.

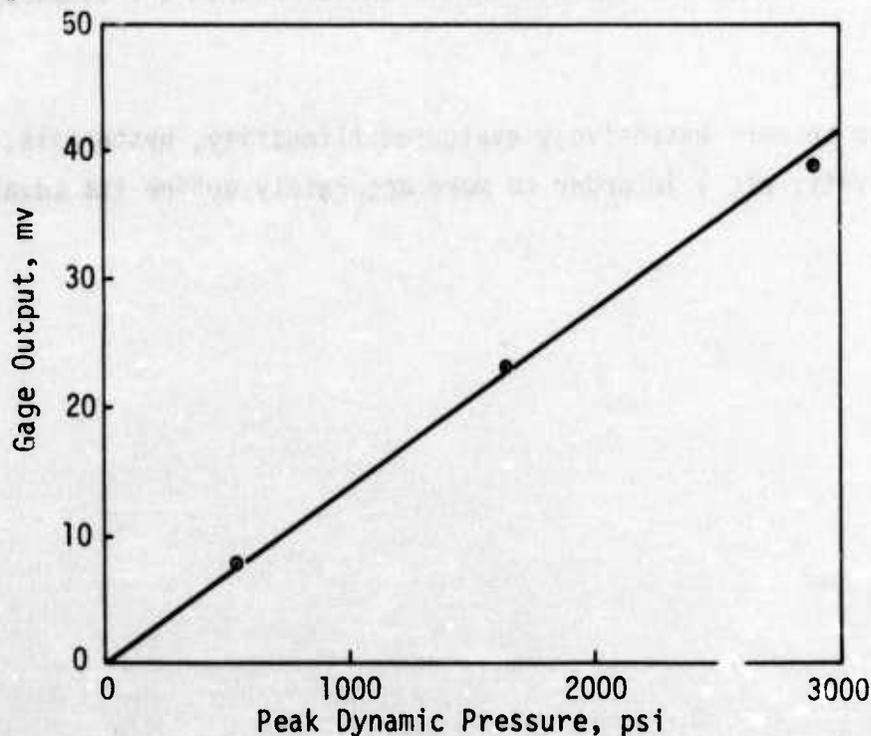


Figure 17. Shock-Tube Calibration of Redesigned Piezoresistive Bar Gage

SECTION V
CONCLUSIONS AND RECOMMENDATIONS

The piezoresistive bar gage damped with beeswax appears to work well, provided the beeswax maintains good contact with the pressure bar. It also appears that filling the gages by the extrusion-filling process assures good contact. The wax-filled bar gage developed here had a fast rise time ($\approx 2 \mu\text{sec}$) and little overshoot and ringing; and from DABS IA experience, it appears to be rugged and reliable.

The acceleration sensitivity of the piezoresistive bar gage is higher than that of some types of diaphragm gages, but not so high as to cause problems in most shock-tube experiments. No noise in the DABS IA data could be attributed to acceleration sensitivity. There may be construction techniques which would reduce the acceleration sensitivity, thus reducing the potential problem.

The zero offsets experienced in DABS IA (a result of the extremely harsh debris environment) can probably be reduced by shielding the pressure bar with a softer material such as lead. Reducing the impact stresses in this manner should reduce or eliminate the inelastic deformation within the steel pressure bar.

The gage needs to be more extensively evaluated (linearity, hysteresis, temperature sensitivity, etc.) in order to more accurately define its advantages and limitations.

DISTRIBUTION LIST

DEPARTMENT OF DEFENSE

Director
Defense Advanced Rsch. Proj. Agency
ATTN: PMO
ATTN: NMRO
ATTN: Tech. Lib.
ATTN: STO

Defense Documentation Center
2 cy ATTN: TC

Director
Defense Nuclear Agency
ATTN: DDST
ATTN: STSI, Archives
ATTN: STAP
2 cy ATTN: SPSS
3 cy ATTN: STTL, Tech. Lib.

Commander
Field Command
Defense Nuclear Agency
ATTN: FCPR
ATTN: FCT
ATTN: FCTMOF

Dir. of Defense Rsch. & Engineering
ATTN: Asst. Dir., Strat. Wpns.

Director
Defense Intelligence Agency
ATTN: DI-7D
ATTN: DI-3

Dir., OSD, ARPA
ATTN: NMR

Ch., LVLO
ATTN: FCTCL

JSTPS
ATTN: JLTW

Chief
Livermore Diviston, Fld. Command, DNA
ATTN: FCPRL

Director
National Security Agency
ATTN: C-513

DEPARTMENT OF THE ARMY

Dep. Chief of Staff for Rsch., Dev. & Acq.
ATTN: Tech. Lib.

Commander
Harry Diamond Laboratories
ATTN: DRXDO-TI, Tech. Lib.
ATTN: DRXDO-NP

Commander
U. S. Army Materiel Dev. & Readiness Cmd.
ATTN: Tech. Lib.

DEPARTMENT OF THE ARMY (Continued)

Director
U. S. Army Ballistic Research Labs.
ATTN: DRXBR-X, Julius J. Meszaros
ATTN: AMXBR-TL-IR, J. H. Keefer
ATTN: Tech. Lib., Edward Balcy
ATTN: AMXER-TB
ATTN: AMXBR-BL
ATTN: AMXBR-RL
ATTN: AMXBR

Director
U. S. Army Engr. Waterways Exper. Sta.
ATTN: Guy Jackson
ATTN: John N. Strange
ATTN: Leo Ingram
ATTN: Tech. Lib.
ATTN: William Flathau
ATTN: WESRL
ATTN: WESSS

U. S. Army Combat Dev. Cmd.

USAMBER&DI
ATTN: SGRD-UBG

USAMC, RSIC
ATTN: Chief, Doc. Sec.
ATTN: SENSC-DB

USABMDPO
ATTN: A. J. Bast, Jr.

USABMDS COM, BMDATC
ATTN: BMDATC-A
ATTN: RDMH-M

CO, Picatinny Arsenal
ATTN: SMUPA-TN
ATTN: AMSMV
ATTN: STINFO Ofc.

CG, WSMR
ATTN: Tech. Lib.

ORDL, CE
ATTN: ORDLBVR

CO, USAEC
ATTN: AMSEL-IO-T
ATTN: AMSEL-XL-S

CO, USARO

Chief of Engineers
ATTN: DAEN-RDM

USA Med. Fld. Svc. Sch.
ATTN: Stimson Lib.

DEPARTMENT OF THE NAVY

Chief of Naval Research
ATTN: Tech. Lib.

DEPARTMENT OF THE NAVY (Continued)

NCEL

Officer-in-Charge
Civil Engineering Laboratory
ATTN: Tech. Lib.
ATTN: R. J. Odello

Commander
Naval Facilities Engineering Command
ATTN: Tech. Lib.

Commander
Naval Ship Engineering Center
ATTN: Tech. Lib.

Commander
Naval Ship Rsch. & Development Ctr.
ATTN: Code L42-3, Library

CO, ESC

Commander
Naval Ship Rsch. & Development Ctr.
ATTN: Tech. Lib.

Commander
Naval Surface Weapons Center
ATTN: Code WX-21, Tech. Lib.
ATTN: Code WA-501, Navy Nuc. Prgms. Off.
ATTN: 730

Chief of Naval Operations

Office of Naval Research
ATTN: 418

Commander
Naval Air Systems Command
ATTN: AIR-52023

Naval Ships Systems Command
ATTN: Lib., NAVSHIPS 08

Director
Naval Research Laboratory
ATTN: 2027

Director
Naval Research Laboratory/EOTPO
ATTN: 5503

Commander
Naval Electronics Laboratory Ctr.
ATTN: 4223

Commander
Naval Weapons Center
ATTN: 753

Director
Special Projects Officer

Ordnance Systems Command

Commanding Officer
Naval Weapons Evaluation Facility
ATTN: ADS

DEPARTMENT OF THE NAVY (Continued)

Officer-in-Charge
Naval Weapons Center

DEPARTMENT OF THE AIR FORCE

AF Geophysics Laboratory, AFSC
ATTN: SUOL, AFCRL, Rsch. Lib.

AF Institute of Technology, AU
ATTN: Library, AFIT, Bldg. 640, Area B
ATTN: CES
ATTN: DAPD

AF Weapons Laboratory, AFSC
ATTN: DES, M. A. Plamondon
ATTN: DEX
ATTN: DED-I, Mr. Santos J. Ayala
ATTN: DES

5 cy ATTN: DED
ATTN: HO, Dr. Minge

ATTN: AL
ATTN: ALC
ATTN: ALE
ATTN: ALO

ATTN: AR
ATTN: DE

ATTN: DY
ATTN: DYS

ATTN: DYT
ATTN: DYV

ATTN: DYX
ATTN: EL

ATTN: ELA
ATTN: ELC

ATTN: ELP
ATTN: ELS

ATTN: LR
ATTN: I

ATTN: LRL
ATTN: LRO

ATTN: LRP
ATTN: PG

ATTN: PGA
ATTN: PGV

ATTN: PO
ATTN: SA

ATTN: SAB
ATTN: SAS

ATTN: SAT
ATTN: SAW

ATTN: SE
ATTN: SEC

ATTN: SEE
ATTN: SES

ATTN: TP
ATTN: IN

2 cy ATTN: SUL

HQ USAF/IN
ATTN: INATA

HQ USAF/PR
ATTN: PREE
ATTN: PREV
ATTN: PREPB

HQ USAF/SA
ATTN: SA
ATTN: SAMI

DEPARTMENT OF THE AIR FORCE (Continued)

HQ USAF/RD
ATTN: RDPQ, 1C370
ATTN: RDQPN, 1D425
ATTN: RDQS

HQ USAF/SG
ATTN: SGPP

HQ USAF/XO
ATTN: XOOWD

AFML
ATTN: Tech. Lib.
ATTN: MX

AWS
ATTN: AWVAS

AFATL
ATTN: DLOSL
ATTN: DEE

RADC
ATTN: Doc. Lib.
ATTN: TUGF

AFRPL
ATTN: DYSN
ATTN: MKCD

ADC
ATTN: ADSWO

SAAMA
ATTN: SE

USAFSAM
ATTN: SUL-4
ATTN: EDAD

TAC
ATTN: DEE

823 CES
ATTN: HR

CINCUSAFE
ATTN: DEE
ATTN: DOA

CINCPACAF
ATTN: DEE
ATTN: DOA

USAF, SCLO
ATTN: Maj Pierson, Chief, LO

AFAPL
ATTN: Tech. Lib.
ATTN: RJL
ATTN: POD

AFLC
ATTN: MMWQ

SACLO

TACLOS

DEPARTMENT OF THE AIR FORCE (Continued)

AFLC
ATTN: DEE

ADC/DE
ATTN: DEE

ADC/DO
ATTN: DOA

ADC/XP
ATTN: XPQDQ
ATTN: XPQY

AUL
ATTN: LDE

AU
ATTN: ED, Dir., Civ. Eng.

AFAL
ATTN: TE

AFISC
ATTN: PQAL
ATTN: SE
ATTN: SEL
ATTN: SEO

USAFA
ATTN: DFSLB
ATTN: FJSRL, CC
ATTN: DFCE

AFSC
ATTN: DO
ATTN: DOB
ATTN: DLSP
ATTN: DLCAW
ATTN: SGB
ATTN: XRP
ATTN: T&E

TAC
ATTN: DEE
ATTN: DERP
ATTN: LGMD
ATTN: SGSB

AFTAC
ATTN: TAP

AFFDL
ATTN: DOO/Lib.
ATTN: STINFO Ofc.

ASD
ATTN: ENYEHM
ATTN: Tech. Lib.
ATTN: DEE

AFOSR
Dir., Nuc. Surety
ATTN: SN

CINCSAC
ATTN: DEE
ATTN: DOXS
ATTN: XPFC

DEPARTMENT OF THE AIR FORCE (Continued)

AFCEC
ATTN: PREC

SAMSO/DE
ATTN: DEE

SAMSO/SE
ATTN: SEN

ESD
ATTN: SE
ATTN: DEE

ENERGY RESEARCH & DEVELOPMENT ADMINISTRATION

University of California
Lawrence Livermore Laboratory
ATTN: Tech. Info., Dept. L-3

University of California
Lawrence Berkeley Laboratory
ATTN: Library

Sandia Laboratories
Livermore Laboratory
ATTN: Doc. Con. for Tech. Lib.

Sandia Laboratories
ATTN: Doc. Con. for Luke J. Vortman
ATTN: Doc. Con. for A. J. Chaban
ATTN: Doc. Con. for Org. 3422-1, Sandia Rpt. Coll.

U. S. Energy Rsch. & Dev. Admin.
Albuquerque Operations Office
ATTN: Doc. Con. for Tech. Lib.

U. S. Energy Rsch. & Dev. Admin.
Division of Headquarters Services
ATTN: Doc. Con. for Class. Tech. Lib.

U. S. Energy Rsch. & Dev. Admin.
Nevada Operations Office
ATTN: Doc. Con. for Tech. Lib.

U. S. Energy Rsch. & Dev. Admin.
Canoga Park Office

Division of Military Application
U. S. Energy Rsch. & Dev. Admin.
ATTN: Dr. Rhodes

Los Alamos Scientific Laboratory
ATTN: Rpt. Lib.

DEPARTMENT OF DEFENSE CONTRACTORS

Aerospace Corporation
ATTN: Tech. Info. Services
ATTN: Prem N. Mathur

Agbabian Associates
ATTN: M. Agbabian

Civil/Nuclear Systems Corp.
ATTN: Robert Crawford

EG&G, Inc.
Albuquerque Division
ATTN: Tech. Lib.

DEPARTMENT OF DEFENSE CONTRACTORS (Continued)

General Electric Company
TEMPO-Center for Advanced Studies
ATTN: DASIAC

IIT Research Institute
ATTN: Tech. Lib.

Kaman Sciences Corporation
ATTN: Library
ATTN: Paul A. Ellis

Merritt Cases, Incorporated
ATTN: Tech. Lib.
ATTN: J. L. Merritt

The Mitre Corporation
ATTN: Library

Nathan M. Newmark
Consulting Engineering Services
ATTN: Nathan M. Newmark

Physics International Company
ATTN: Doc. Con. for Tech. Lib.
ATTN: Doc. Con. for Charles Godfrey
ATTN: Doc. Con. for Coye Vincent
ATTN: Doc. Con. for Fred M. Sauer

R & D Associates
ATTN: Bruce Hartenbaum
ATTN: Tech. Lib.
ATTN: J. G. Lewis

Science Applications, Inc.
ATTN: Michael McKay
ATTN: Tech. Lib.

Science Applications, Inc.
ATTN: R. A. Shunk

Southwest Research Institute
ATTN: A. B. Wenzel
ATTN: Wilfred E. Baker

Stanford Research Institute
ATTN: George R. Abrahamson
ATTN: Carl Peterson
ATTN: Burt R. Gasten

Systems, Science & Software, Inc.
ATTN: Tech. Lib.
ATTN: Donald R. Grine

TRW Systems Group
ATTN: Tech. Info. Ctr., S-1930
2 cy ATTN: Peter K. Dai, R1-2170

TRW Systems Group
San Bernardino Operations
ATTN: E. Y. Wong, 527/712

The Eric H. Wang Civil Engineering Rsch. Fac.
ATTN: Kenneth B. Simmons

The University of New Mexico
ATTN: Larry Bickle
ATTN: Neal Baum

DEPARTMENT OF DEFENSE CONTRACTORS (Continued)

Weidlinger Assoc. Consulting Engineers
ATTN: Melvin L. Baron

DEPARTMENT OF DEFENSE CONTRACTORS (Continued)

Weidlinger Assoc. Consulting Engineers
ATTN: J. Isenberg

THIS REPORT HAS BEEN DELIMITED
AND CLEARED FOR PUBLIC RELEASE
UNDER DOD DIRECTIVE 5200.20 AND
NO RESTRICTIONS ARE IMPOSED UPON
ITS USE AND DISCLOSURE.

DISTRIBUTION STATEMENT A

APPROVED FOR PUBLIC RELEASE,
DISTRIBUTION UNLIMITED.