

# CELLULAR GENOMIC ANALYSIS WITH GMR SENSOR ARRAYS

C.R. Tamanaha<sup>1</sup>, S.P. Mulvaney<sup>1</sup>, K.A. Wahowski<sup>2</sup>,  
M.C. Tondra<sup>3</sup>, L.J. Whitman<sup>1</sup>, R.J. Colton<sup>1</sup>

<sup>1</sup>Naval Research Laboratory, Washington, DC 20375

<sup>2</sup>Nova Research, Inc., Alexandria, VA 22308

<sup>3</sup>NVE Corporation, Eden Prairie, MN 55344

## ABSTRACT

A new cellular genomic analysis device is introduced that integrates cell lysing, microfluidics, and micromagnetic mRNA labeling and detection on one microfabricated substrate. The magnetic sensor, benzocyclobutene (BCB) microfluidics, investigative genomic assay, magnetic labels, and surface chemistry development for the new cellular genomic analysis device are described.

**KEYWORDS:** biosensor, genomics, GMR, magnetic labeling

## 1. INTRODUCTION

A number of issues hinder the genomic analysis of heterogeneous mixtures of cells. For example, current gene array technologies perform poorly when screening a low cell population. This limitation becomes even more relevant when dealing with the quantification of very low mRNA copy numbers per cell [1]. We have previously developed a unique DNA hybridization detection system that relies on giant magnetoresistive (GMR) sensors [2,3]. This system, based on the detection of magnetic microbead labels, is capable of observing a single DNA hybridization event. We are now attempting to apply this technology to the detection of low concentrations of mRNA, ideally that from a single cell.

## Report Documentation Page


*Form Approved*  
*OMB No. 0704-0188*

Public reporting burden for the collection of information is estimated to average 1 hour per response, including the time for reviewing instructions, searching existing data sources, gathering and maintaining the data needed, and completing and reviewing the collection of information. Send comments regarding this burden estimate or any other aspect of this collection of information, including suggestions for reducing this burden, to Washington Headquarters Services, Directorate for Information Operations and Reports, 1215 Jefferson Davis Highway, Suite 1204, Arlington VA 22202-4302. Respondents should be aware that notwithstanding any other provision of law, no person shall be subject to a penalty for failing to comply with a collection of information if it does not display a currently valid OMB control number.


1. REPORT DATE <b>2003</b>	2. REPORT TYPE	3. DATES COVERED <b>00-00-2003 to 00-00-2003</b>	
4. TITLE AND SUBTITLE <b>Cellular Genomic Analysis with GMR Sensor Arrays</b>		5a. CONTRACT NUMBER	
		5b. GRANT NUMBER	
		5c. PROGRAM ELEMENT NUMBER	
6. AUTHOR(S)		5d. PROJECT NUMBER	
		5e. TASK NUMBER	
		5f. WORK UNIT NUMBER	
7. PERFORMING ORGANIZATION NAME(S) AND ADDRESS(ES) <b>Naval Research Laboratory, 4555 Overlook Avenue SW, Washington, DC, 20375</b>		8. PERFORMING ORGANIZATION REPORT NUMBER	
9. SPONSORING/MONITORING AGENCY NAME(S) AND ADDRESS(ES)		10. SPONSOR/MONITOR'S ACRONYM(S)	
		11. SPONSOR/MONITOR'S REPORT NUMBER(S)	
12. DISTRIBUTION/AVAILABILITY STATEMENT <b>Approved for public release; distribution unlimited</b>			
13. SUPPLEMENTARY NOTES <b>7th International Conference on Miniaturized Chemical and Biochemical Analysts Systems, October 5-9, 2003, Squaw Valley, CA</b>			
14. ABSTRACT <b>A new cellular genomic analysis device is introduced that integrates cell lysing microfluidics, and micromagnetic mRNA labeling and detection on one microfabricated substrate. The magnetic sensor, benzocyclobutene (BCB) microfluidics, investigative genomic assay, magnetic labels, and surface chemistry development for the new cellular genomic analysis device are described.</b>			
15. SUBJECT TERMS			
16. SECURITY CLASSIFICATION OF:			17. LIMITATION OF ABSTRACT
a. REPORT <b>unclassified</b>	b. ABSTRACT <b>unclassified</b>	c. THIS PAGE <b>unclassified</b>	<b>Same as Report (SAR)</b>
			18. NUMBER OF PAGES <b>4</b>
			19a. NAME OF RESPONSIBLE PERSON

## 2. DEVICE DESIGN

A unique microchip has been fabricated that includes dual field-in-plane excited spin-valve GMR sensors, microfluidic channels with a cross-sectional area approximately  $140 \mu\text{m}^2$ , and micron-scale lysing electrodes (based on Figure 1). The fluidic channels are

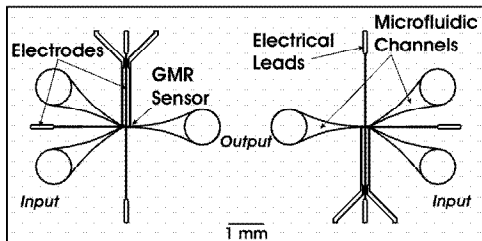

**Figure 1.** The layout of a GMR sensor chip with integrated microfluidic channels and lysing electrodes. The GMR sensor is approximately  $180 \mu\text{m}$  long (not visible at this scale).



**Figure 2.** Two-layer BCB polymer microfluidic channels. The image is centered at the junction of the cell lysing and genetic detection zones.

built up from two layers of benzocyclobutene (BCB), a commonly used photosensitive polymer used in the electronics industry (Figure 2), and later sealed with a poly(dimethylsiloxane) (PDMS) cap. The fluidic system contains two distinct zones through which biological samples will be processed: 1) isolation/lysing and 2) genetic detection. The isolation/lysing zone contains a pair of electrodes at which individual cells can be electronically lysed using a series of high current density voltage pulses. The cell lysing region is connected to the labeling and genetic detection region by a shallow "filter" that is about  $2 \mu\text{m}$  deep. For genome analysis, immobilized DNA or peptide nucleic acid (PNA) probes will cover the GMR sensors to create a planar capture surface.

Detection of genomic material occurs at a single GMR resistor that spans the entire detection region. The detection region is defined by microfluidic channels covering the

GMR chip surface. The detection region is about 10  $\mu\text{m}$  wide by 180  $\mu\text{m}$  long by 14  $\mu\text{m}$  high. There is an identical reference resistor adjacent to the sense resistor that is not under the flow channel. It is expected that the detector will be able to see the entire range of 1 to 500 magnetic beads immobilized on its surface (based on 2.8  $\mu\text{m}$  diameter commercial magnetic beads). The linear, low-hysteresis GMR sensing material is made using the following basic structure (listed from bottom to top, all dimensions in nm):

**Ta 4 / NiFeCo 5 / Ta 5 / NiFeCo 4 / CoFe 1 / Cu 2.5 / CoFe 42 / CrPtMn 32.5.**

This magnetoresistive material design generates about 5% resistance change over a range of +/- 20 Oe. (Several annealing steps are required to get ideal sensing behavior from these sensors.) The GMR sensors are covered with a 200 nm layer of  $\text{Si}_3\text{N}_4$  for electrical isolation, and then common microfabrication techniques are used to form Al connections from the GMR sensors to bonding pads.

### 3. SUPPORTING EXPERIMENTS

*Assay development.* In preparation for examination of mRNA in raw yeast cell samples, we have developed reliable protocols with commercially available mouse brain and *Saccharomyces cerevisiae* poly(A)<sup>+</sup> RNA samples. These experiments are also leading to a calibration system that will be used to corroborate mRNA capture and detection via GMR sensing of magnetic beads. In addition, we plan to use these “idealized” samples of poly(A)<sup>+</sup> RNA to prove that our sensor is capable of low mRNA abundance detection without RT-PCR.

*Magnetic microbead label development.* Small lots of NiFe powder were vigorously shaken over a polycarbonate filter (5  $\mu\text{m}$  pore) for several hours. The collected beads showed a tight distribution with an average diameter of 1  $\mu\text{m}$ . Beads were coated with aminopropyltrimethoxy silane under drop-wise addition to a vigorously stirred solution. The amine-terminated beads were reacted with NHS-PEG-vinyl sulfone. Thiolated antibodies attach to the vinyl sulfone terminus to produce the conjugated magnetic bead.

*Sensor substrate surface chemistry development.* It was determined that more repeatable results are obtained for nucleic acid assays when using alumina rather than Au films as an immobilization substrate. The number of primary amines available after the addition of polyethyleneimine (PEI) and the number of vinyl sulfone (VS) groups present after the subsequent reaction with NHS-PEG-VS are very consistent when utilizing evaporated alumina layers. In addition, a blocking strategy involving the combination of casein and Tween® 20 has proven to be the most effective against non-specific binding of streptavidin-conjugated beads on the VS terminated surfaces.

#### **4. CONCLUSIONS**

A new GMR sensor and integrated BCB microfluidic channel design has been fabricated. In conjunction with supporting genomic assay, magnetic label, and biologically compatible sensor substrate surface chemistry development, this cellular genomic analysis system shows the promise of achieving the high sensitivity necessary for low mRNA abundance detection without RT-PCR.

#### **ACKNOWLEDGEMENTS**

This work has been supported by ONR, NIH/BECON and NIGMS, DOE, and DARPA.

#### **REFERENCES**

- [1] J.F. Leary, *Enabling Molecular Profiling with Cellular Resolution: Microgenomics using Homogeneous Cell Samples*, San Diego, CA (December 5-6, 2002).
- [2] R.L. Edelstein, C.R. Tamanaha, P.E. Sheehan, M.M. Miller, D.R. Baselt, L.J. Whitman, and R.J. Colton, *Biosens. Bioelectron.* **14**, 805-813 (2000).
- [3] C.R. Tamanaha, L.J. Whitman, and R.J. Colton, *J. Micromech. Microeng.*, **12**, N7–N17 (2002).